


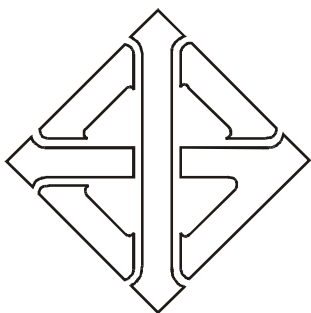

มาตรฐานผลิตภัณฑ์อุตสาหกรรม

THAI INDUSTRIAL STANDARD

มอก. 1441 เล่ม 1–2548

CISPR 16–1–1(2003–11)

ข้อกำหนดสำหรับอุปกรณ์และวิธีการวัดสัญญาณ รบกวนวิทยุและภูมิคุ้มกัน

เล่ม 1–1 อุปกรณ์วัดสัญญาณรบกวนวิทยุและภูมิคุ้มกัน – อุปกรณ์วัด

SPECIFICATION FOR RADIO DISTURBANCE AND IMMUNITY

MEASURING APPARATUS AND METHODS–

PART 1–1 : RADIO DISTURBANCE AND IMMUNITY MEASURING APPARATUS–MEASURING
APPARATUS

สำนักงานมาตรฐานผลิตภัณฑ์อุตสาหกรรม

กระทรวงอุตสาหกรรม

ICS 33.100

ISBN 974-1508-20-4

มาตรฐานผลิตภัณฑ์อุตสาหกรรม
ข้อกำหนดสำหรับอุปกรณ์และวิธีการวัดสัญญาณ
รบกวนวิทยุและภูมิคุ้มกัน

เล่ม 1-1 อุปกรณ์วัดสัญญาณรบกวนวิทยุและภูมิคุ้มกัน – อุปกรณ์วัด

มอก. 1441 เล่ม 1-2548

สำนักงานมาตรฐานผลิตภัณฑ์อุตสาหกรรม
กระทรวงอุตสาหกรรม ถนนพระรามที่ 6 กรุงเทพฯ 10400
โทรศัพท์ 0 2202 3300

ประกาศในราชกิจจานุเบกษาฉบับประกาศและงานทั่วไป เล่ม 123 ตอนที่ 83ง
วันที่ 24 สิงหาคม พุทธศักราช 2549

บริษัทไฟฟ้าและอิเล็กทรอนิกส์ตลอดจนบริษัทเทคโนโลยีสารสนเทศในขณะใช้งานจะต้องไม่ส่งสัญญาณรบกวนเข้าสู่ระบบไฟฟ้าหรือรบกวนการทำงานของบริษัทข้างเคียง รวมทั้งตัวบริษัทเองก็ต้องมีภูมิคุ้มกันในระดับเพียงพอที่จะทำงานในสภาวะแวดล้อมทางแม่เหล็กไฟฟ้าในระดับหนึ่งได้ จึงกำหนดมาตรฐานผลิตภัณฑ์อุตสาหกรรม ข้อกำหนดสำหรับอุปกรณ์และวิธีการวัดสัญญาณรบกวนวิทยุและภูมิคุ้มกัน เล่ม 1-1 อุปกรณ์วัดสัญญาณรบกวนวิทยุและภูมิคุ้มกัน □
อุปกรณ์วัด ขึ้น

มาตรฐานผลิตภัณฑ์อุตสาหกรรมนี้กำหนดขึ้นโดยรับ CISPR 16-1-1 (2003-11) Specification for radio disturbance and immunity measuring apparatus and methods – Part 1-1 : Radio disturbance and immunity measuring apparatus – Measuring apparatus มาใช้ในระดับเหมือนกันทุกประการ (identical) โดยใช้ CISPR ฉบับภาษาอังกฤษเป็นหลัก

มาตรฐานผลิตภัณฑ์อุตสาหกรรมนี้กำหนดขึ้นเพื่อใช้ในการอ้างอิง และเพื่อให้ทันกับความต้องการของผู้ใช้มาตรฐาน ซึ่งจะได้แปลเป็นภาษาไทยในโอกาสอันสมควรต่อไป หากมีข้อสงสัยโปรดติดต่อสอบถามสำนักงานมาตรฐานผลิตภัณฑ์อุตสาหกรรม

คณะกรรมการมาตรฐานผลิตภัณฑ์อุตสาหกรรมได้พิจารณามาตรฐานนี้แล้ว เห็นสมควรเสนอรัฐมนตรีประกาศตาม มาตรา 15 แห่งพระราชบัญญัติมาตรฐานผลิตภัณฑ์อุตสาหกรรม พ.ศ. 2511



ประกาศกระทรวงอุตสาหกรรม

ฉบับที่ 3493 (พ.ศ. 2549)

ออกตามความในพระราชบัญญัติมาตรฐานผลิตภัณฑ์อุตสาหกรรม

พ.ศ. 2511

เรื่อง ยกเลิกมาตรฐานผลิตภัณฑ์อุตสาหกรรม

อุปกรณ์และวิธีการวัดสัญญาณรบกวนวิทยุและภูมิคุ้มกัน

เล่ม 1 อุปกรณ์วัดสัญญาณรบกวนวิทยุและภูมิคุ้มกัน

และกำหนดมาตรฐานผลิตภัณฑ์อุตสาหกรรม

ข้อกำหนดสำหรับอุปกรณ์และวิธีการวัดสัญญาณรบกวนวิทยุและภูมิคุ้มกัน

เล่ม 1-1 อุปกรณ์วัดสัญญาณรบกวนวิทยุและภูมิคุ้มกัน-อุปกรณ์วัด

โดยที่เป็นการสมควรปรับปรุงมาตรฐานผลิตภัณฑ์อุตสาหกรรม อุปกรณ์และวิธีการวัดสัญญาณรบกวนวิทยุและภูมิคุ้มกัน เล่ม 1 อุปกรณ์วัดสัญญาณรบกวนวิทยุและภูมิคุ้มกัน มาตรฐานเลขที่ มอก. 1441-2545

อาศัยอำนาจตามความในมาตรา 15 แห่งพระราชบัญญัติมาตรฐานผลิตภัณฑ์อุตสาหกรรม พ.ศ. 2511 รัฐมนตรีว่าการกระทรวงอุตสาหกรรมออกประกาศยกเลิกประกาศกระทรวงอุตสาหกรรม ฉบับที่ 3143 (พ.ศ. 2546) ออกตามความในพระราชบัญญัติมาตรฐานผลิตภัณฑ์อุตสาหกรรม พ.ศ. 2511 เรื่อง กำหนดมาตรฐานผลิตภัณฑ์อุตสาหกรรม อุปกรณ์และวิธีการวัดสัญญาณรบกวนวิทยุและภูมิคุ้มกัน เล่ม 1 อุปกรณ์วัดสัญญาณรบกวนวิทยุและภูมิคุ้มกัน ลงวันที่ 13 มิถุนายน พ.ศ. 2546 และออกประกาศกำหนดมาตรฐานผลิตภัณฑ์อุตสาหกรรม ข้อกำหนดสำหรับอุปกรณ์และวิธีการวัดสัญญาณรบกวนวิทยุและภูมิคุ้มกัน เล่ม 1-1 อุปกรณ์วัดสัญญาณรบกวนวิทยุและภูมิคุ้มกัน-อุปกรณ์วัด มาตรฐานเลขที่ มอก. 1441 เล่ม 1-2548 ขึ้นใหม่ ดังมีรายละเอียดต่อท้ายประกาศนี้

ทั้งนี้ให้มีผลตั้งแต่วันที่ประกาศในราชกิจจานุเบกษา เป็นต้นไป

ประกาศ ณ วันที่ 26 เมษายน พ.ศ. 2549

สุริยะ จึงรุ่งเรืองกิจ

รัฐมนตรีว่าการกระทรวงอุตสาหกรรม

มาตรฐานผลิตภัณฑ์อุตสาหกรรม

ข้อกำหนดสำหรับอุปกรณ์และวิธีการวัดสัญญาณรบกวนวิทยุและภูมิคุ้มกัน

เล่ม 1-1 อุปกรณ์วัดสัญญาณรบกวนวิทยุและภูมิคุ้มกัน - อุปกรณ์วัด

มาตรฐานผลิตภัณฑ์อุตสาหกรรมนี้กำหนดขึ้นโดยรับ CISPR 16-1-1(2003-11) Specification for radio disturbance and immunity measuring apparatus and methods - Part 1-1 : Radio disturbance and immunity measuring apparatus - Measuring apparatus มาใช้ในระดับเหมือนกันทุกประการ(identical) โดยใช้ CISPR ฉบับภาษาอังกฤษเป็นหลัก

มาตรฐานผลิตภัณฑ์อุตสาหกรรมนี้ได้รับการระบุให้เป็นมาตรฐานพื้นฐาน ซึ่งกำหนดลักษณะเฉพาะและสมรรถนะของบริภัณฑ์สำหรับวัดแรงดันไฟฟ้ารบกวนวิทยุ กระแสไฟฟ้ารบกวนวิทยุ และสนามรบกวนวิทยุ ในพิสัยความถี่ 9 กิโลเฮิร์ตซ์ ถึง 18 จิกะเฮิร์ตซ์

นอกจากนี้ข้อกำหนดยังระบุไว้สำหรับบริภัณฑ์พิเศษสำหรับการวัดสัญญาณรบกวนไม่ต่อเนื่อง รวมทั้งการวัดสัญญาณรบกวนวิทยุแถบความถี่กว้างและแถบความถี่แคบ

แบบของเครื่องรับที่ครอบคลุมรวมถึง

- เครื่องรับสำหรับวัดค่ายอดเสมือน
- เครื่องรับสำหรับวัดค่ายอด
- เครื่องรับสำหรับวัดค่าเฉลี่ย
- เครื่องรับสำหรับวัดค่ารากกำลังสองเฉลี่ย

นอกจากนี้ยังมีข้อกำหนดสำหรับเครื่องวิเคราะห์สเปกตรัม เครื่องรับกราดตรวจ และโวลต์มิเตอร์ความถี่เสียง

คุณลักษณะที่ต้องการตามมาตรฐานเล่มนี้ต้องเป็นไปตามที่กำหนดที่ทุกความถี่และทุกระดับแรงดันไฟฟ้ารบกวนวิทยุ กระแสไฟฟ้ารบกวนวิทยุ และกำลังไฟฟ้ารบกวนวิทยุ หรือความแรงสนามรบกวนวิทยุ ภายในพิสัยแสดงค่าของบริภัณฑ์วัด

วิธีการวัดครอบคลุมโดยเล่ม 2 และสารสนเทศเพิ่มเติมเกี่ยวกับสัญญาณรบกวนวิทยุให้ไว้ในเล่ม 3 ความไม่แน่นอน สถิติ และการทำแบบขีดจำกัด ครอบคลุมโดยเล่ม 4

รายละเอียดให้เป็นไปตาม CISPR 16-1-1 (2003-11)

CONTENTS

FOREWORD	5
INTRODUCTION	5
TABLE RECAPITULATING CROSS-REFERENCES	6
 1 Scope	 7
2 Normative references	7
3 Definitions	9
4 Quasi-peak measuring receivers for the frequency range 9 kHz to 1 000 MHz	11
5 Peak measuring receivers for the frequency range 9 kHz to 1 000 MHz	23
6 Average measuring receivers for the frequency range 9 kHz to 1 000 MHz	25
7 RMS measuring receivers for the frequency range 9 kHz to 1 000 MHz	28
8 Spectrum analyzers and scanning receivers	30
9 Audio-frequency voltmeter	32
10 Disturbance analyzers	36
 Annex A (normative) Determination of response to repeated pulses of quasi-peak and r.m.s. measuring receivers (subclauses 3.2, 4.4.2, 7.2.2 and 7.4.1)	 45
Annex B (normative) Determination of pulse generator spectrum (subclauses 4.4, 5.4, 6.4, 7.4)	50
Annex C (normative) Accurate measurements of the output of nanosecond pulse generators (subclauses 4.4, 5.4, 6.4, 7.4)	52
Annex D (normative) Influence of the quasi-peak measuring receiver characteristics on its pulse response (subclause 4.4.2)	54
Annex E (normative) Response of average and peak measuring receivers (subclause 6.2.1)	55
Annex F (normative) Performance check of the exceptions from the definitions of a click according to 4.2.3 of CISPR 14-1	59

INTERNATIONAL ELECTROTECHNICAL COMMISSION
INTERNATIONAL SPECIAL COMMITTEE ON RADIO INTERFERENCE

**SPECIFICATION FOR RADIO DISTURBANCE AND IMMUNITY
MEASURING APPARATUS AND METHODS –**

**Part 1-1: Radio disturbance and immunity measuring apparatus –
Measuring apparatus**

FOREWORD

- 1) The International Electrotechnical Commission (IEC) is a worldwide organization for standardization comprising all national electrotechnical committees (IEC National Committees). The object of IEC is to promote international co-operation on all questions concerning standardization in the electrical and electronic fields. To this end and in addition to other activities, IEC publishes International Standards, Technical Specifications, Technical Reports, Publicly Available Specifications (PAS) and Guides (hereafter referred to as "IEC Publication(s)"). Their preparation is entrusted to technical committees; any IEC National Committee interested in the subject dealt with may participate in this preparatory work. International, governmental and non-governmental organizations liaising with the IEC also participate in this preparation. IEC collaborates closely with the International Organization for Standardization (ISO) in accordance with conditions determined by agreement between the two organizations.
- 2) The formal decisions or agreements of IEC on technical matters express, as nearly as possible, an international consensus of opinion on the relevant subjects since each technical committee has representation from all interested IEC National Committees.
- 3) IEC Publications have the form of recommendations for international use and are accepted by IEC National Committees in that sense. While all reasonable efforts are made to ensure that the technical content of IEC Publications is accurate, IEC cannot be held responsible for the way in which they are used or for any misinterpretation by any end user.
- 4) In order to promote international uniformity, IEC National Committees undertake to apply IEC Publications transparently to the maximum extent possible in their national and regional publications. Any divergence between any IEC Publication and the corresponding national or regional publication shall be clearly indicated in the latter.
- 5) IEC provides no marking procedure to indicate its approval and cannot be rendered responsible for any equipment declared to be in conformity with an IEC Publication.
- 6) All users should ensure that they have the latest edition of this publication.
- 7) No liability shall attach to IEC or its directors, employees, servants or agents including individual experts and members of its technical committees and IEC National Committees for any personal injury, property damage or other damage of any nature whatsoever, whether direct or indirect, or for costs (including legal fees) and expenses arising out of the publication, use of, or reliance upon, this IEC Publication or any other IEC Publications.
- 8) Attention is drawn to the Normative references cited in this publication. Use of the referenced publications is indispensable for the correct application of this publication.
- 9) Attention is drawn to the possibility that some of the elements of this IEC Publication may be the subject of patent rights. IEC shall not be held responsible for identifying any or all such patent rights.

International Standard CISPR 16-1-1 has been prepared by CISPR subcommittee A: Radio interference measurements and statistical methods.

This first edition of CISPR 16-1-1, together with CISPR 16-1-2, CISPR 16-1-3, CISPR 16-1-4 and CISPR 16-1-5, cancels and replaces the second edition of CISPR 16-1, published in 1999, amendment 1 (2002) and amendment 2 (2003). It contains the relevant clauses of CISPR 16-1 without technical changes.


This publication has been drafted in accordance with the ISO/IEC Directives, Part 2.

The committee has decided that the contents of this publication will remain unchanged until 2004. At this date, the publication will be

- reconfirmed;
- withdrawn;
- replaced by a revised edition, or
- amended.

INTRODUCTION

CISPR 16-1, CISPR 16-2, CISPR 16-3 and CISPR 16-4 have been reorganised into 14 parts, to accommodate growth and easier maintenance. The new parts have also been renumbered. See the list given below.

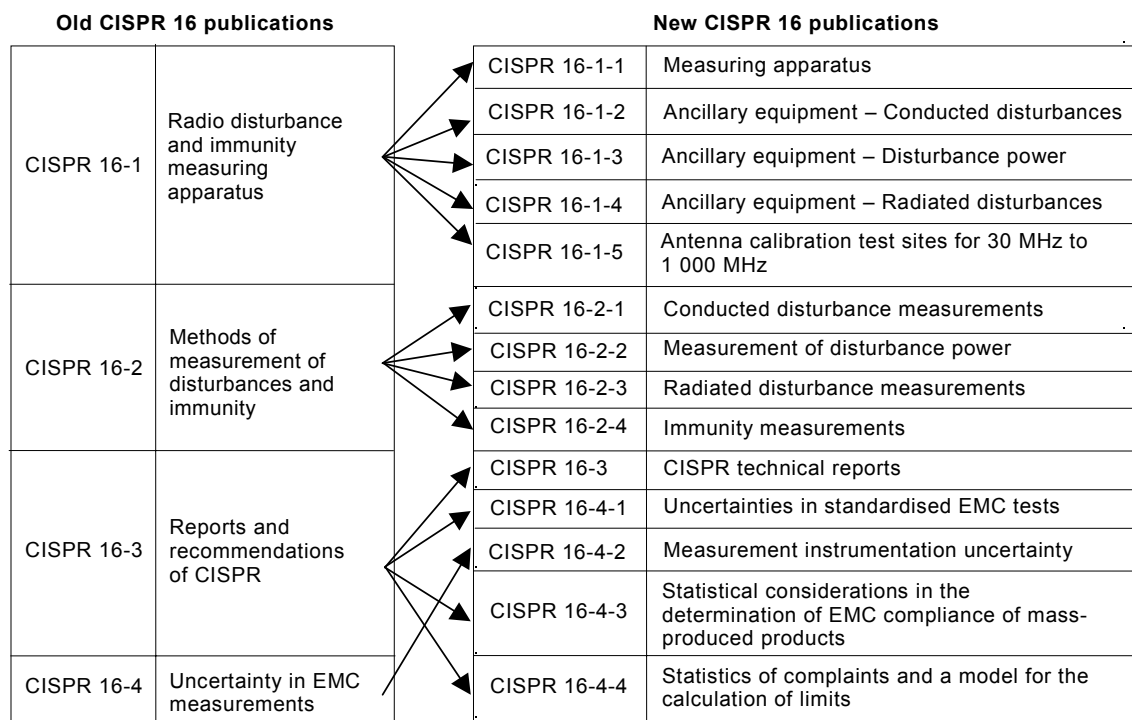

More specific information on the relation between the 'old' CISPR 16-1 and the present 'new' CISPR 16-1-1 is given in the table after this introduction (TABLE RECAPITULATING CROSS REFERENCES).

Measurement instrumentation specifications are given in five new parts of CISPR 16-1, while the methods of measurement are covered now in four new parts of CISPR 16-2. Various reports with further information and background on CISPR and radio disturbances in general are given in CISPR 16-3. CISPR 16-4 contains information related to uncertainties, statistics and limit modelling.

CISPR 16-1 consists of the following parts, under the general title *Specification for radio disturbance and immunity measuring apparatus and methods – Radio disturbance and immunity measuring apparatus*:

Part 1-1: Measuring apparatus,

Part 1-2: Ancillary equipment – Conducted disturbances,

Part 1-3: Ancillary equipment – Disturbance power,

Part 1-4: Ancillary equipment – Radiated disturbances,

Part 1-5: Antenna calibration test sites for 30 MHz to 1 000 MHz.

TABLE RECAPITULATING CROSS-REFERENCES

Second edition of CISPR 16-1

Clauses, subclauses

1

2

3

4.1

4.2

4.3

4.4

4.5

4.6

5.4

Annexes

A

B

C

D

E

Y

Figures

1,...,3

60, 61

4,...,6

11, 12

21, 22

First edition of CISPR 16-1-1

Clauses, subclauses

1

2

3

4

5

6

7

8

9

10

Annexes

A

B

C

D

E

F

Figures

1,...,3

4, 5

6,...,8

9, 10

E.1, E.2

SPECIFICATION FOR RADIO DISTURBANCE AND IMMUNITY MEASURING APPARATUS AND METHODS –

Part 1-1: Radio disturbance and immunity measuring apparatus – Measuring apparatus

1 Scope

This part of CISPR 16 is designated a basic standard, which specifies the characteristics and performance of equipment for the measurement of radio disturbance voltages, currents and fields in the frequency range 9 kHz to 18 GHz. In addition, requirements are specified for specialized equipment for discontinuous disturbance measurements. The requirements include the measurement of broadband and narrowband types of radio disturbance.

The receiver types covered include the following:

- a) the quasi-peak measuring receiver,
- b) the peak measuring receiver,
- c) the average measuring receiver,
- d) the r.m.s. measuring receiver.

In addition there are specifications for spectrum analyzers, scanning receivers and audio-frequency voltmeters.

The requirements of this publication shall be complied with at all frequencies and for all levels of radio disturbance voltages, currents, power or field strengths within the CISPR indicating range of the measuring equipment.

Methods of measurement are covered in Part 2, and further information on radio disturbance is given in Part 3 of CISPR 16. Uncertainties, statistics and limit modelling are covered in Part 4 of CISPR 16.

2 Normative references

The following referenced documents are indispensable for the application of this document. For dated references, only the edition cited applies. For undated references, the latest edition of the referenced document (including any amendments) applies.

CISPR 11:2003, *Industrial, scientific and medical (ISM) radio-frequency equipment – Electro-magnetic disturbance characteristics – Limits and methods of measurement*

CISPR 14-1:2000, *Electromagnetic compatibility – Requirements for household appliances, electric tools and similar apparatus – Part 1: Emission*

CISPR 16-1-2:2003, *Specification for radio disturbance and immunity measuring apparatus and methods – Part 1-2: Radio disturbance and immunity measuring apparatus – Ancillary equipment – Conducted disturbances*

CISPR 16-1-3:2003, *Specification for radio disturbance and immunity measuring apparatus and methods – Part 1-3: Radio disturbance and immunity measuring apparatus – Ancillary equipment – Disturbance power*

CISPR 16-1-4:2003, *Specification for radio disturbance and immunity measuring apparatus and methods – Part 1-4: Radio disturbance and immunity measuring apparatus – Ancillary equipment - Radiated disturbances*

CISPR 16-1-5:2003, *Specification for radio disturbance and immunity measuring apparatus and methods – Part 1-5: Radio disturbance and immunity measuring apparatus – Antenna calibration test sites for 30 MHz to 1 000 MHz*

CISPR 16-2-1:2003, *Specification for radio disturbance and immunity measuring apparatus and methods – Part 2-1: Methods of measurement of immunity and disturbance – Conducted disturbance measurements*

CISPR 16-2-2:2003, *Specification for radio disturbance and immunity measuring apparatus and methods – Part 2-2: Methods of measurement of immunity and disturbance – Measurement of disturbance power*

CISPR 16-2-3:2003, *Specification for radio disturbance and immunity measuring apparatus and methods – Part 2-3: Methods of measurement of immunity and disturbance – Radiated disturbance measurements*

CISPR 16-2-4:2003, *Specification for radio disturbance and immunity measuring apparatus and methods – Part 2-4: Methods of measurement of immunity and disturbance – Immunity measurements*

CISPR 16-3:2003, *Specification for radio disturbance and Immunity measuring apparatus and methods – Part 3: CISPR technical reports*

CISPR 16-4-1:2003, *Specification for radio disturbance and immunity measuring apparatus and methods – Part 4-1: Uncertainties, statistics and limit modelling – Uncertainties in standardized EMC tests*

CISPR 16-4-2:2003, *Specification for radio disturbance and immunity measuring apparatus and methods – Part 4-2: Uncertainties, statistics and limit modelling – Measurement instrumentation uncertainty*

CISPR 16-4-3:2003, *Specification for radio disturbance and immunity measuring apparatus and methods – Part 4-3: Uncertainties, statistics and limit modelling – Statistical considerations in the determination of EMC compliance of mass-produced products*

CISPR 16-4-4:2003, *Specification for radio disturbance and immunity measuring apparatus and methods – Part 4-4: Uncertainties, statistics and limit modelling – Statistics of complaints and a model for the calculation of limits*

IEC 60050(161):1990, *International Electrotechnical Vocabulary (IEV) – Chapter 161: Electromagnetic compatibility*
Amendment 1:1997 and Amendment 2:1998

IEC 60315-3:1999, *Methods of measurement or radio receivers for various classes of emissions – Part 3: Receivers for amplitude-modulated sound-broadcasting emissions*

IEC 60315-4:1997, *Methods of measurement or radio receivers for various classes of emissions – Part 4: Radio-frequency measurements on receivers for frequency modulated sound-broadcasting emissions*

ITU-R Recommendation BS.468-4:1986, *Measurement of audio-frequency noise voltage level in sound broadcasting*

ITU-T Recommendation P. 53 of *Blue Book* (1989), Volume V – *Psophometers (apparatus for the objective measurement of circuit noise)*. See also ITU-R Rec. O.41 (10/94).

International Vocabulary of Basic and General Terms in Metrology, International Organization for Standardization, Geneva, 2nd edition, 1993

3 Definitions

For the purpose of this part of CISPR 16, the following definitions apply. Also see IEC 60050 (161).

3.1

bandwidth (B_n)

the width of the overall selectivity curve of the receiver between two points at a stated attenuation, below the midband response. The bandwidth is represented by the symbol B_n , where n is the stated attenuation in decibels.

3.2

impulse bandwidth (B_{imp})

$$B_{\text{imp}} = A(t)_{\text{max}} / (2 G_o \times IS)$$

where

$A(t)_{\text{max}}$ is the peak of the envelope at the IF output of the receiver with an impulse area IS applied at the receiver input;

G_o is the gain of the circuit at the centre frequency.

Specifically for two critically-coupled tuned transformers,

$$B_{\text{imp}} = 1,05 \times B_6 = 1,31 \times B_3$$

where

B_6 and B_3 are respectively the bandwidths at the –6 dB and –3 dB points (see clause A.2 in annex A for further information).

3.3

impulse area (IS)

the impulse area (sometimes called impulse strength, IS) is the voltage-time area of a pulse defined by the integral:

$$IS = \int_{-\infty}^{+\infty} V(t) dt \text{ (expressed in } \mu\text{Vs or dB}(\mu\text{Vs))}$$

NOTE Spectral density (D) is related to impulse area and expressed in $\mu\text{V/MHz}$ or $\text{dB}(\mu\text{V/MHz})$. For rectangular impulses of pulse duration T at frequencies $f \ll 1/T$, the relationship $D (\mu\text{V/MHz}) = 2 \times 10^6 IS (\mu\text{Vs})$ applies.

3.4

electrical charge time constant (T_c)

the time needed after the instantaneous application of a constant sine-wave voltage to the stage immediately preceding the input of the detector for the output voltage of the detector to reach 63 % of its final value

NOTE This time constant is determined as follows: A sine-wave signal of constant amplitude and having a frequency equal to the mid-band frequency of the i.f. amplifier is applied to the input of the stage immediately preceding the detector. The indication, D , of an instrument having no inertia (e.g., a cathode-ray oscilloscope) connected to a terminal in the d.c. amplifier circuit so as not to affect the behaviour of the detector, is noted. The level of the signal is chosen such that the response of the stages concerned remains within the linear operating range. A sine-wave signal of this level, applied for a limited time only and having a wave train of rectangular envelope is gated such that the deflection registered is 0,63D. The duration of this signal is equal to the charge time of the detector.

3.5**electrical discharge time constant (T_D)**

the time needed after the instantaneous removal of a constant sine-wave voltage applied to the stage immediately preceding the input of the detector for the output of the detector to fall to 37 % of its initial value

NOTE The method of measurement is analogous to that for the charge time constant, but instead of a signal being applied for a limited time, the signal is interrupted for a definite time. The time taken for the deflection to fall to 0,37D is the discharge time constant of the detector.

3.6**mechanical time constant (T_M) of a critically damped indicating instrument**

$$T_M = T_L / 2\pi$$

where

T_L is the period of free oscillation of the instrument with all damping removed.

NOTE 1 For a critically damped instrument, the equation of motion of the system may be written as:

$$T_M^2 (d^2\alpha / dt^2) + 2T_M (d\alpha / dt) + \alpha = ki$$

where

α is the deflection;

i is the current through the instrument;

k is a constant.

It can be deduced from this relation that this time constant is also equal to the duration of a rectangular pulse (of constant amplitude) that produces a deflection equal to 35 % of the steady deflection produced by a continuous current having the same amplitude as that of the rectangular pulse.

NOTE 2 The methods of measurement and adjustment are deduced from one of the following:

- The period of free oscillation having been adjusted to $2\pi T_M$, damping is added so that $\alpha T = 0,35\alpha_{\max}$.
- When the period of oscillation cannot be measured, the damping is adjusted to be just below critical such that the overshoot is not greater than 5 % and the moment of inertia of the movement is such that $\alpha T = 0,35\alpha_{\max}$.

3.7**overload factor**

the ratio of the level that corresponds to the range of practical linear function of a circuit (or a group of circuits) to the level that corresponds to full-scale deflection of the indicating instrument

The maximum level at which the steady-state response of a circuit (or group of circuits) does not depart by more than 1 dB from ideal linearity defines the range of practical linear function of the circuit (or group of circuits).

3.8**symmetric voltage**

in a two-wire circuit, such as a single-phase mains supply, the symmetric voltage is the radio-frequency disturbance voltage appearing between the two wires. This is sometimes called the differential mode voltage. If V_a is the vector voltage between one of the mains terminals and earth and V_b is the vector voltage between the other mains terminal and earth, the symmetric voltage is the vector difference ($V_a - V_b$)

3.9**CISPR indicating range**

it is the range specified by the manufacturer which gives the maximum and the minimum meter indications within which the receiver meets the requirements of this section of CISPR 16

4 Quasi-peak measuring receivers for the frequency range 9 kHz to 1 000 MHz

The receiver specification depends on the frequency of operation. There is one receiver specification covering the frequency range 9 kHz to 150 kHz (band A), one covering 150 kHz to 30 MHz (band B), one covering 30 MHz to 300 MHz (band C), and one covering 300 MHz to 1 000 MHz (band D).

4.1 Input impedance

The input circuit of measuring receivers shall be unbalanced. For receiver control settings within the CISPR indicating range, the input impedance shall be nominally 50 Ω with a v.s.w.r. not to exceed 2,0 to 1 when the RF attenuation is 0 and 1,2 to 1 when the RF attenuation is 10 dB or greater.

Symmetric input impedance in the frequency range 9 kHz to 30 MHz: to permit symmetrical measurements a balanced input transformer is used. The preferred input impedance for the frequency range 9 kHz to 150 kHz is 600 Ω . This symmetric input impedance may be incorporated either in the relevant symmetrical artificial network necessary to couple to the receiver or optionally in the measuring receiver.

4.2 Fundamental characteristics

The responses to pulses as specified in 4.4 are calculated on the basis of the measuring receivers having the following fundamental characteristics.

Table 1 – Fundamental characteristics of quasi-peak receivers

Characteristics	Frequency band		
	Band A 9 kHz to 150 kHz	Band B 0,15 MHz to 30 MHz	Bands C and D 30 MHz to 1 000 MHz
Bandwidth at the –6 dB points, B_6 in kHz	0,20	9	120
Detector electrical charge time constant, in ms	45	1	1
Detector electrical discharge time constant, in ms	500	160	550
Mechanical time constant of critically damped indicating instrument, in ms	160	160	100
Overload factor of circuits preceding the detector, in dB	24	30	43,5
Overload factor of the d.c. amplifier between detector and indicating instrument, in dB	6	12	6
NOTE 1 The definition of mechanical time constant (see 3.6) assumes that the indicating instrument is linear, i.e., equal increments of current produce equal increments of deflection. An indicating instrument having a different relation between current and deflection may be used provided that the instrument satisfies the requirements of this subclause. In an electronic instrument, the mechanical time-constant may be simulated by a circuit.			
NOTE 2 No tolerance is given for the electrical and mechanical time constants. The actual values used in a specific receiver will be determined by the design to meet the requirements in 4.4			

4.3 Sine-wave voltage accuracy

The accuracy of measurement of sine-wave voltages shall be better than ± 2 dB when supplied with a sine-wave signal at 50 Ω resistance source impedance.

4.4 Response to pulses

NOTE Annexes B and C describe methods for determining the output characteristics of a pulse generator for use in testing the requirements of this subclause.

4.4.1 Amplitude relationship (absolute calibration)

The response of the measuring receiver to pulses of impulse area of a) μVs (microvolt second) e.m.f. at 50 Ω source impedance, having a uniform spectrum up to at least b) MHz, repeated at a frequency of c) Hz shall, for all frequencies of tuning, be equal to the response to an unmodulated sine-wave signal at the tuned frequency having an e.m.f. of r.m.s. value 2 mV (66 dB(μV)). The source impedances of the pulse generator and the signal generator shall both be the same. A tolerance of $\pm 1,5$ dB shall be permitted on the sine-wave voltage level.


NOTE A lower impulse area may be used together with a proportionally lower amplitude for the unmodulated sinewave input, provided sufficient signal-to-noise ratio is maintained.

Table 2 – Test pulse characteristics for quasi-peak measuring receivers

Frequency range	a) μVs	b) MHz	c) Hz
9 kHz to 150 kHz	13,5	0,15	25
0,15 MHz to 30 MHz	0,316	30	100
30 MHz to 300 MHz	0,044	300	100
300 MHz to 1 000 MHz	0,044	1 000	100


4.4.2 Variation with repetition frequency (relative calibration)

The response of the measuring receiver to repeated pulses shall be such that for a constant indication on the measuring receiver, the relationship between amplitude and repetition frequency is in accordance with figures 1a, 1b or 1c.

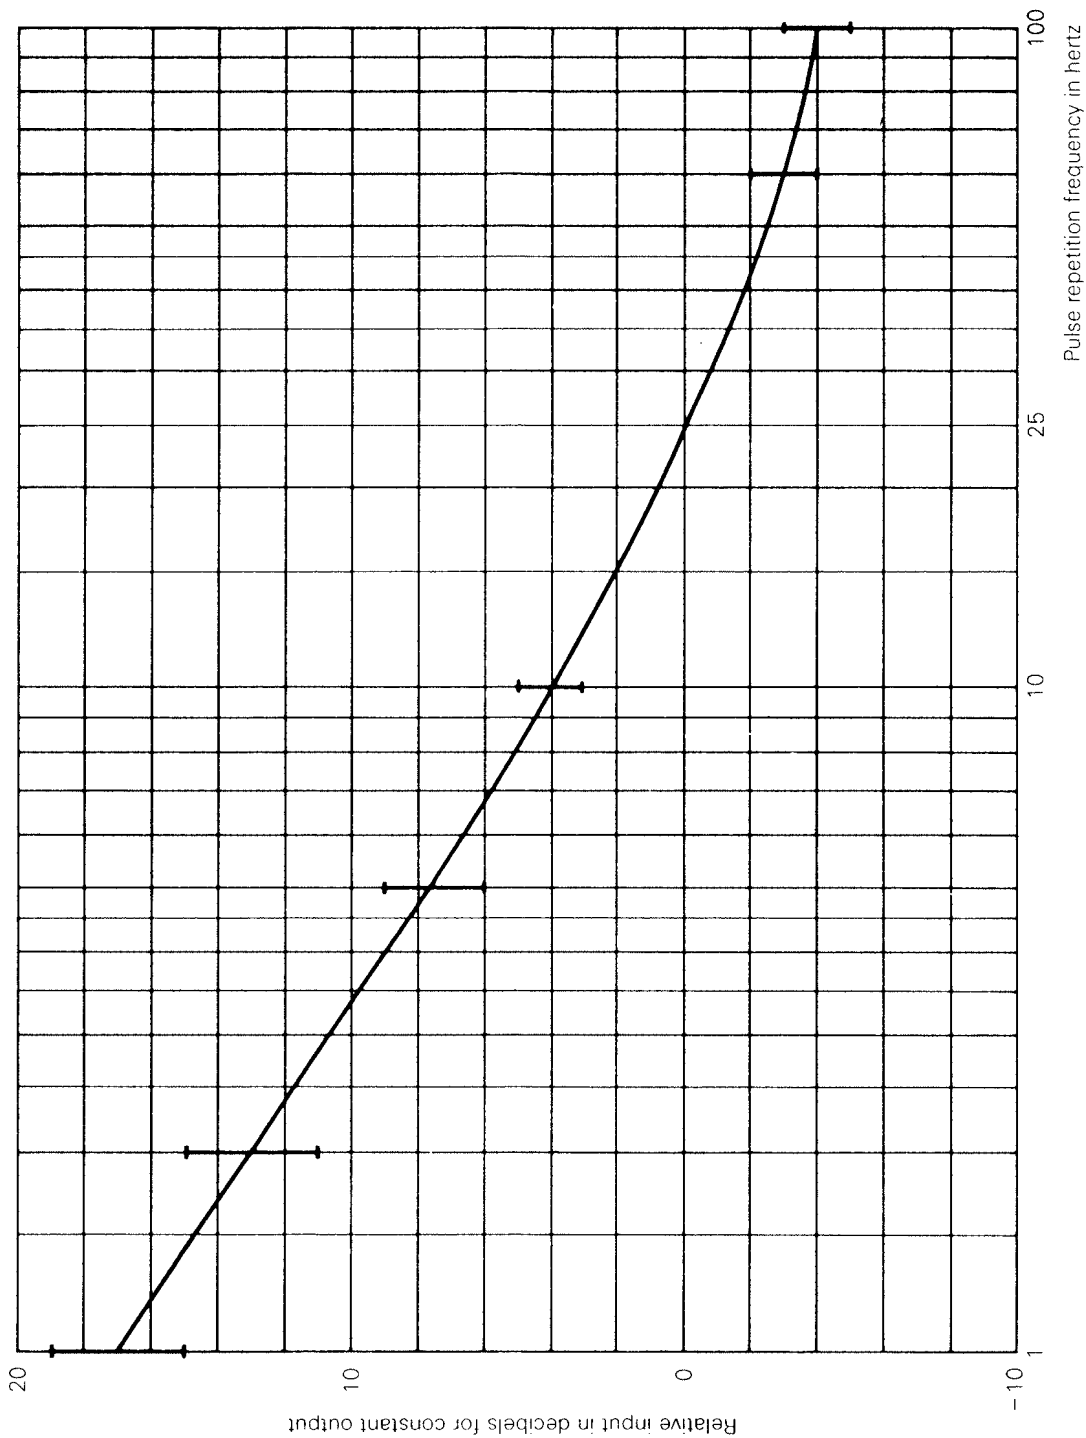

IEC 1290/99

Figure 1a – Pulse response curve (Band A)

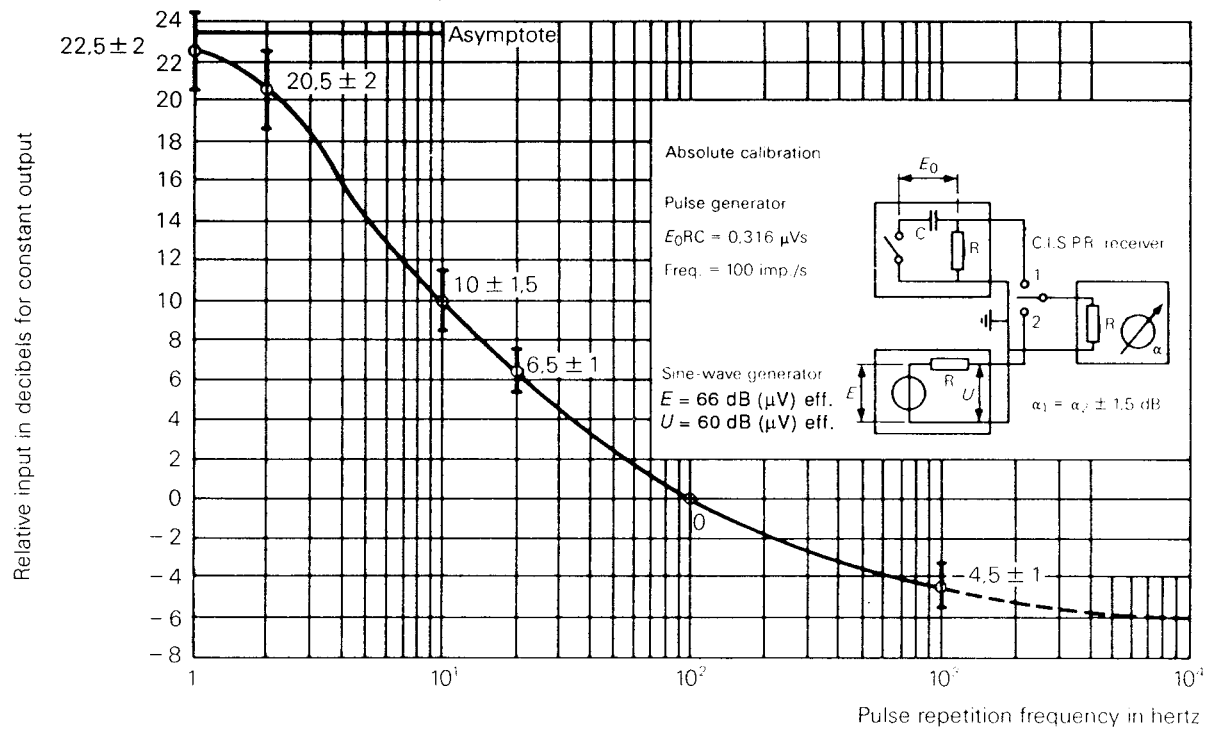

IEC 1291/99

Figure 1b – Pulse response curve (Band B)

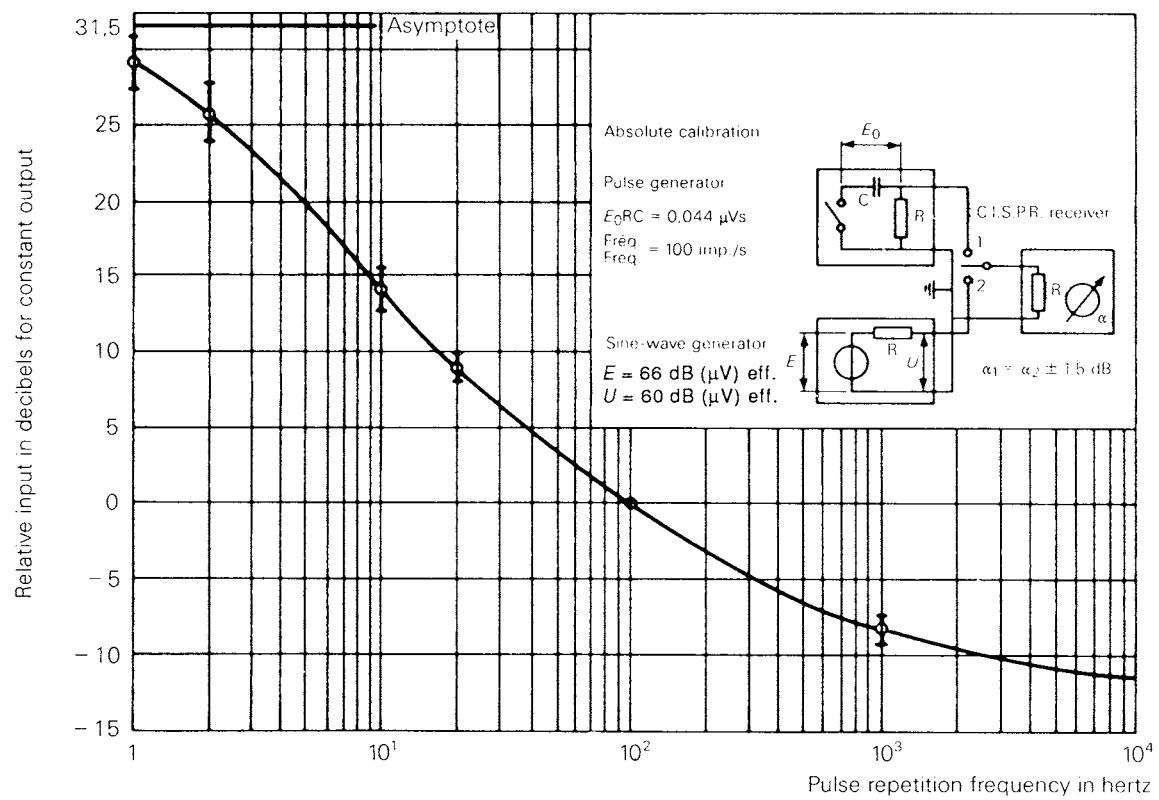


Figure 1c – Pulse response curve (Bands C and D)

The response curve for a particular measuring receiver shall lie between the limits defined in the appropriate figure and quantified in table 3.

Table 3 – Pulse response of quasi-peak receivers

Repetition frequency Hz	Relative equivalent level in dB of pulse for stated band			
	Band A 9 kHz to 150 kHz	Band B 0,15 MHz to 30 MHz	Band C 30 MHz to 300 MHz	Band D 300 MHz to 1 000 MHz
1 000	Note 4	$-4,5 \pm 1,0$	$-8,0 \pm 1,0$	$-8,0 \pm 1,0$
100	$-4,0 \pm 1,0$	0 (ref.)	0 (ref.)	0 (ref.)
60	$-0,3 \pm 1,0$	–	–	–
25	0 (ref.)	–	–	–
20	–	$+6,5 \pm 1,0$	$+9,0 \pm 1,0$	$+9,0 \pm 1,0$
10	$+4,0 \pm 1,0$	$+10,0 \pm 1,5$	$+14,0 \pm 1,5$	$+14,0 \pm 1,5$
5	$+7,5 \pm 1,0$	–	–	–
2	$+13,0 \pm 2,0$	$+20,5 \pm 2,0$	$+26,0 \pm 2,0$	$+26,0 \pm 2,0^*$
1	$+17,0 \pm 2,0$	$+22,5 \pm 2,0$	$+28,5 \pm 2,0$	$+28,5 \pm 2,0^*$
Isolated pulse	$+19,0 \pm 2,0$	$+23,5 \pm 2,0$	$+31,5 \pm 2,0$	$+31,5 \pm 2,0^*$

NOTE 1 The influence of the receiver characteristics upon its pulse response is considered in annex D.


NOTE 2 The relationships between the pulse responses of a quasi-peak receiver and receivers with other detector types are given in 5.4, 6.4.1 and 7.4.1.

NOTE 3 The theoretical pulse response curves of quasi-peak and average detector receivers combined on an absolute scale are shown in figure 1d. The ordinate of figure 1d shows the open-circuit impulse areas in dB(μ Vs) corresponding to the open-circuit sine-wave voltage of 66 dB(μ V) r.m.s. The indication on a measuring receiver with an input matched to the calibrating generators will then be 60 dB(μ V). Where the measuring bandwidth is less than the pulse repetition frequency, the curves of figure 1d are valid when the receiver is tuned to a discrete line of the spectrum.

NOTE 4 It is not possible to specify a response above 100 Hz in the frequency range 9 kHz to 150 kHz because of the overlapping of pulses in the i.f. amplifier.

NOTE 5 Annex A deals with the determination of the curve of response to repeated pulses.

NOTE 6 The pulse response is restricted due to overload at the input to the receiver at frequencies above 300 MHz. The values marked with an asterisk (*) in the table are optional and are not essential.

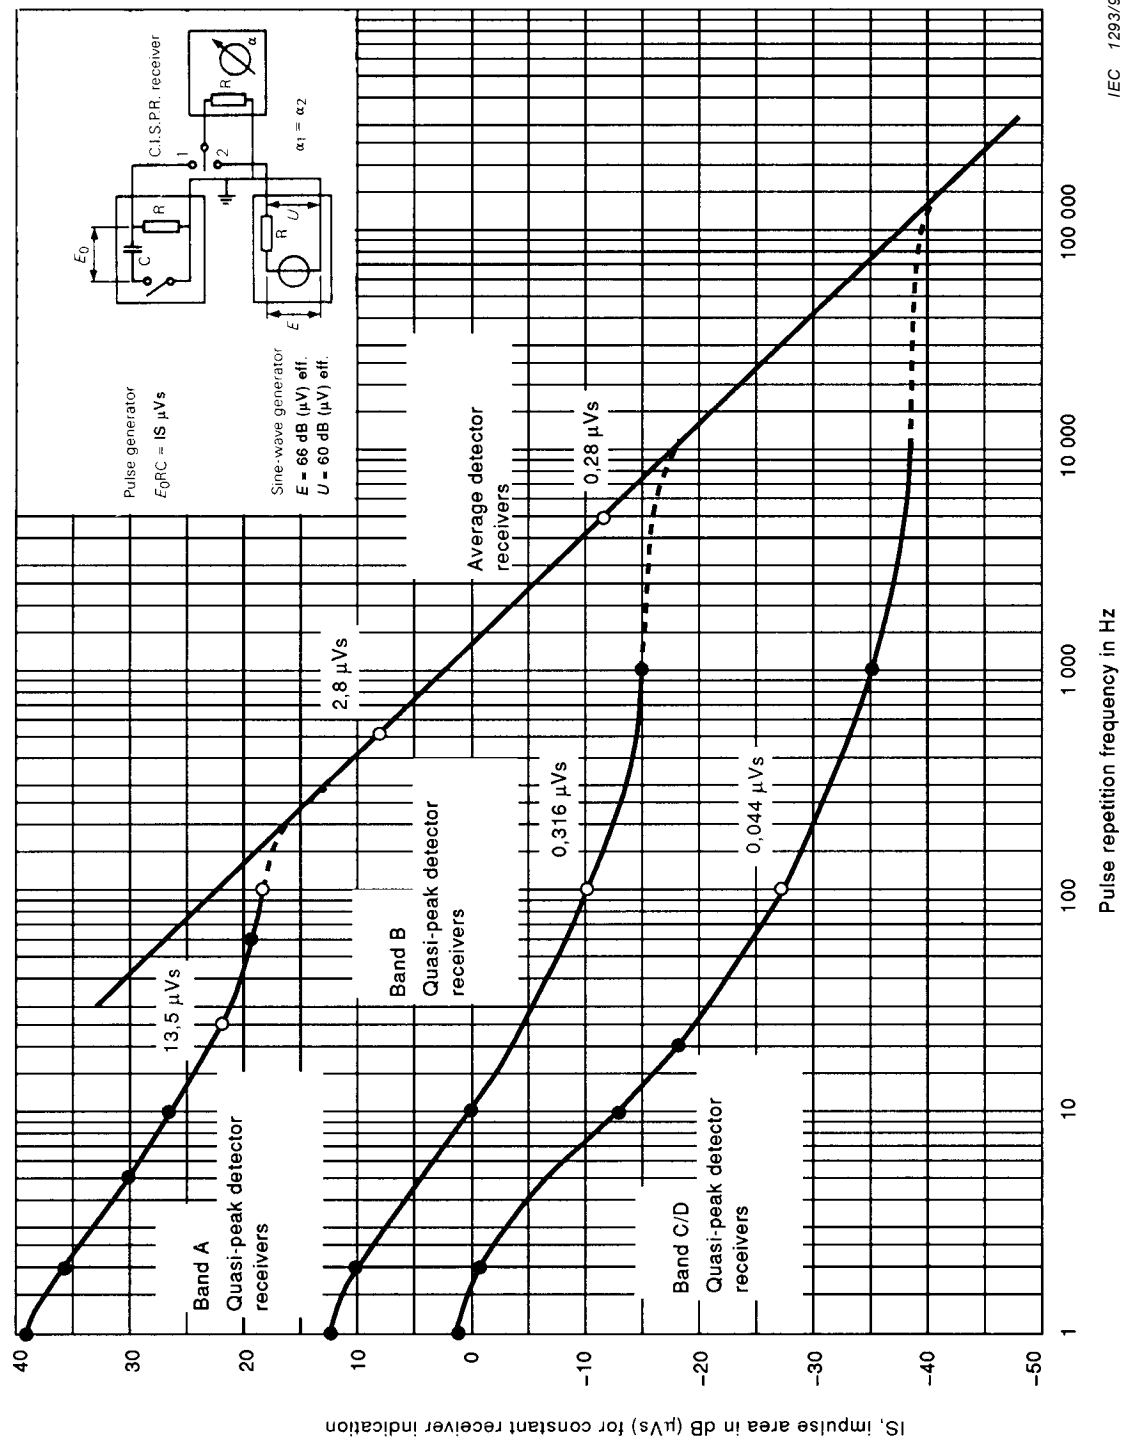

IEC 1293/99

Figure 1d – Theoretical pulse response curve of quasi-peak detector receivers and average detector receiver (see 6.4.2)

4.5 Selectivity

4.5.1 Overall selectivity (passband)

The curve representing the overall selectivity of the measuring receiver shall lie within the limits shown in figures 2a, 2b or 2c.

Selectivity shall be described by the variation with frequency of the amplitude of the input sine-wave voltage that produces a constant indication on the measuring receiver.

NOTE For the measurement of equipment that requires higher selectivity at the transition between 130 kHz and 150 kHz (e.g. mains signalling equipment as defined in EN 50065-1/A2), a highpass filter may be added in front of the measuring receiver to achieve the following combined selectivity of CISPR measuring receiver and highpass filter:

Frequency kHz	Relative attenuation dB
150	≤ 1
146	≤ 6
145	≥ 6
140	≥ 34
130	≥ 81


The measuring receiver in conjunction with the highpass filter should fulfil the requirements of this standard.

4.5.2 Intermediate frequency rejection ratio


The ratio of the input sine-wave voltage at the intermediate frequency to that at the tuned frequency that produces the same indication of the measuring receiver shall be not less than 40 dB. Where more than one intermediate frequency is used, this requirement shall be met at each intermediate frequency.

4.5.3 Image frequency rejection ratio

The ratio of the input sine-wave voltage at the image frequency to that at the tuned frequency that produces the same indication on the measuring receiver shall be not less than 40 dB. Where more than one intermediate frequency is used, this requirement shall be met at the image frequencies corresponding to each intermediate frequency.

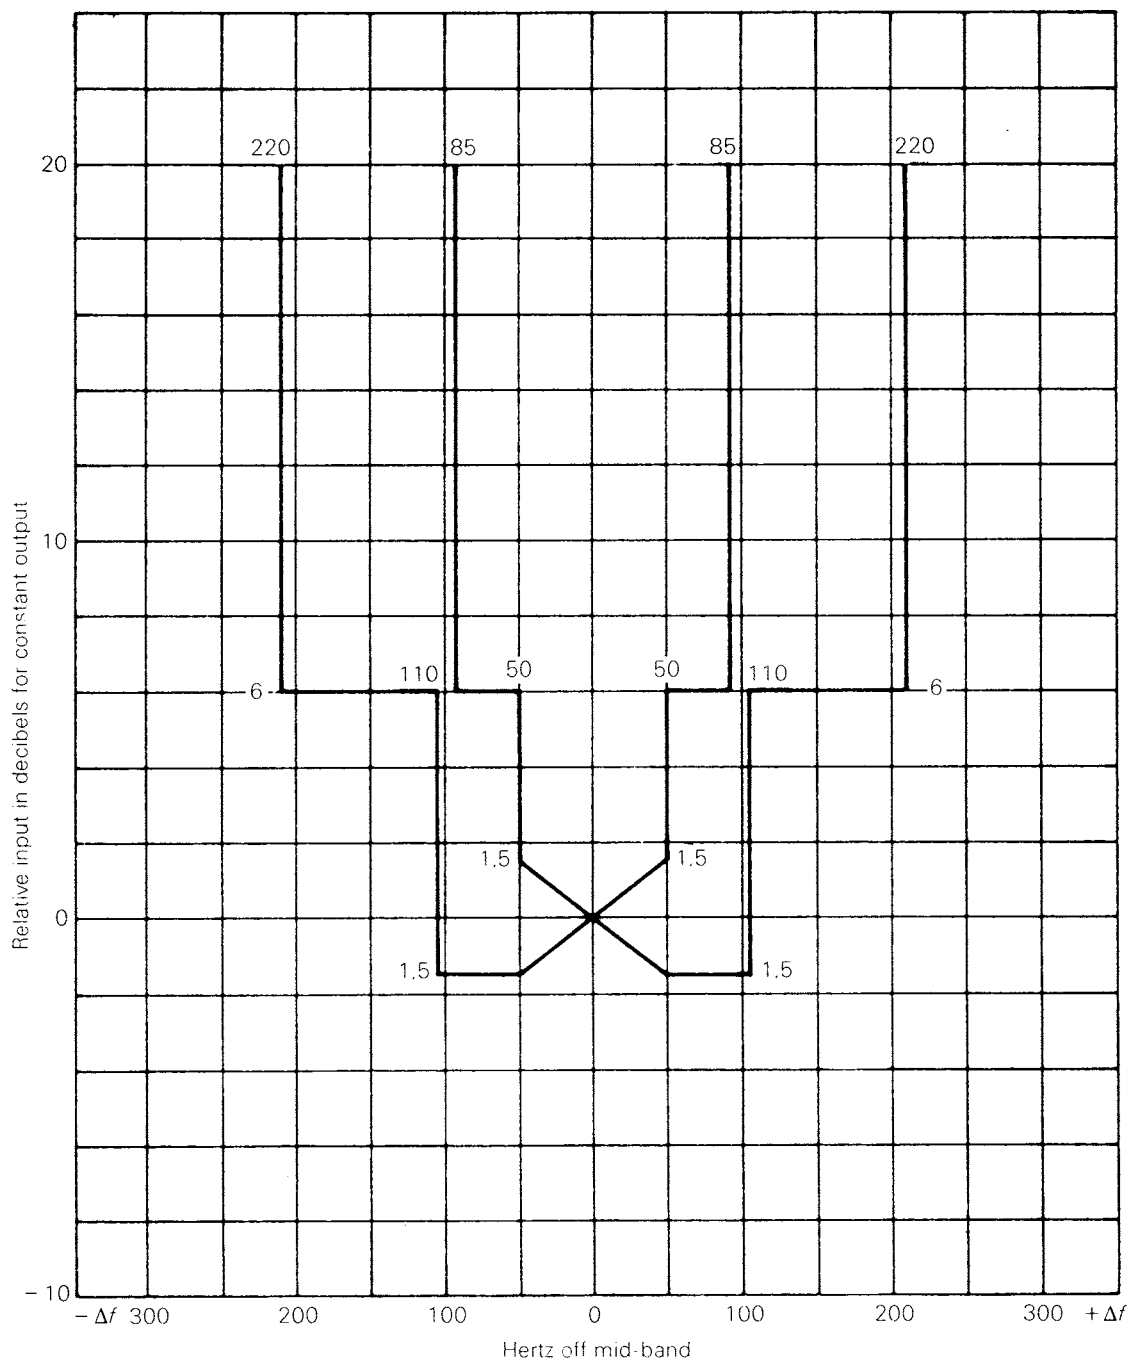


**Figure 2a – Limits of overall selectivity – pass-band
(see 4.5.1, 5.5, 6.5, 7.5) (Band A)**

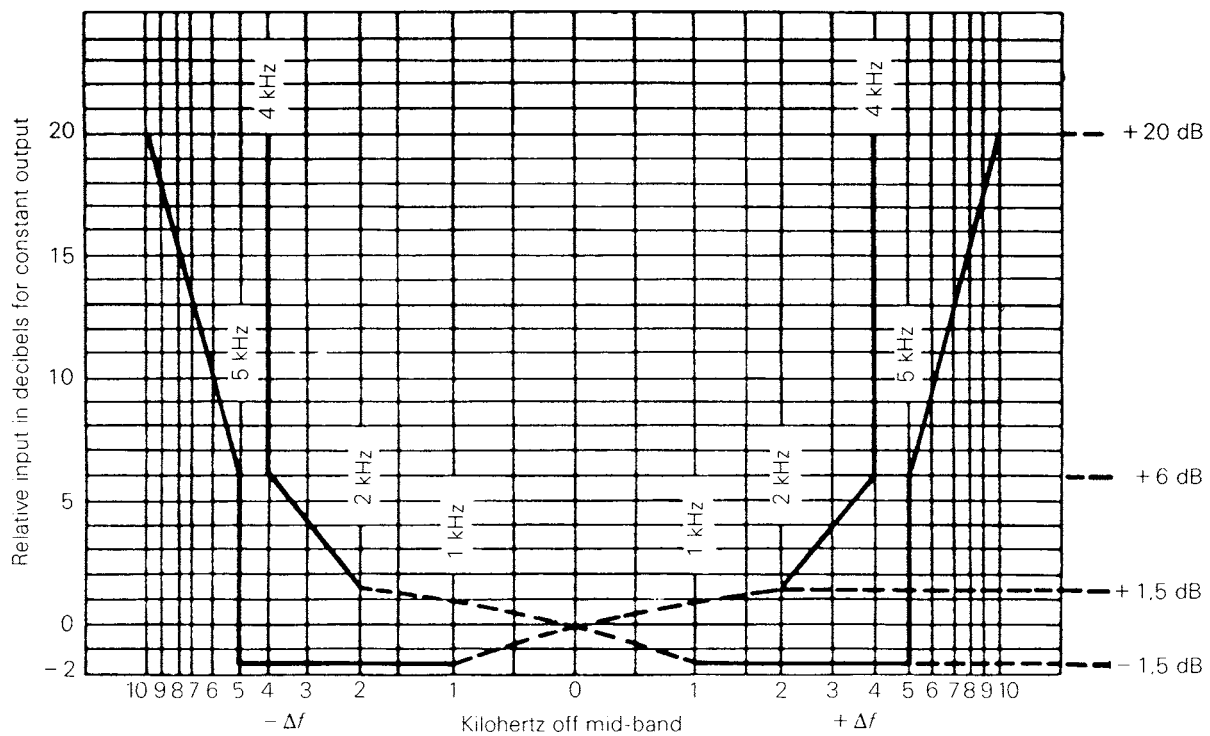

IEC 1295/99

Figure 2b – Limits of overall selectivity – pass-band (see 4.5.1, 5.5, 6.5) (Band B)

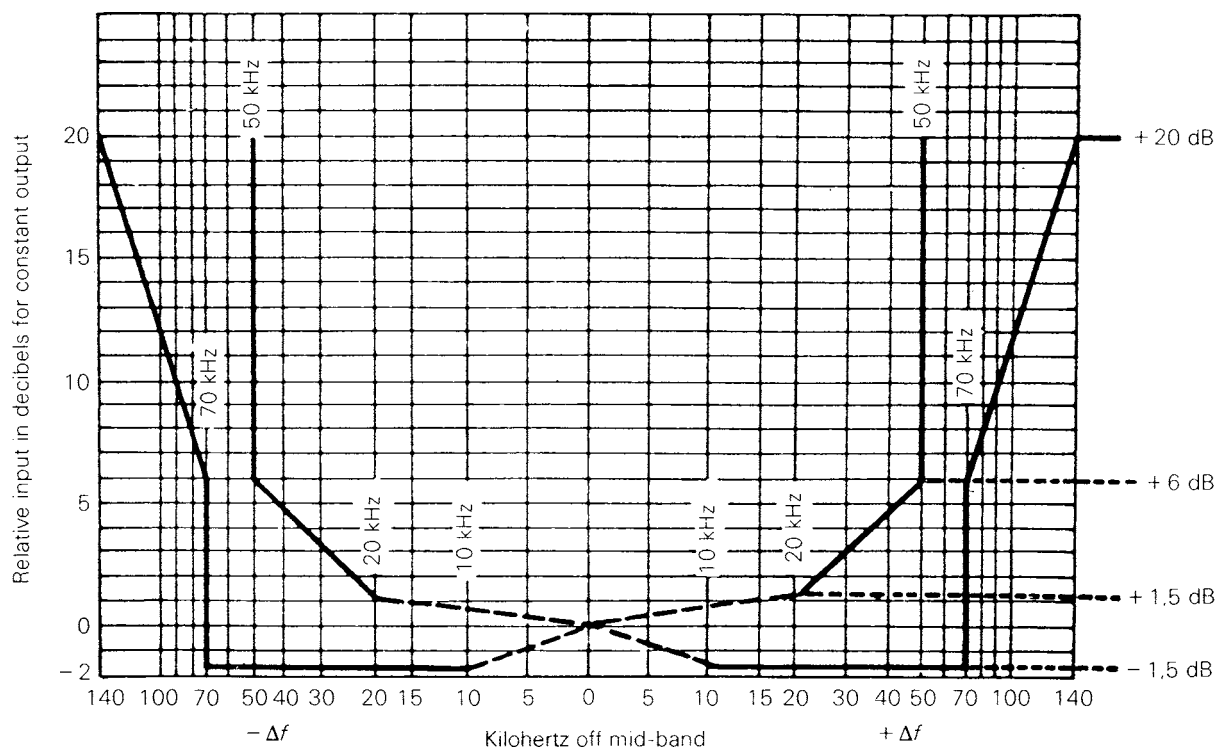

IEC 1296/99

Figure 2c – Limits of overall selectivity – pass-band (see 4.5.1, 5.5, 6.5, 7.5) (Bands C and D)

4.5.4 Other spurious responses

The ratio of the input sine-wave voltage at frequencies other than those specified in 4.5.2 and 4.5.3 to that at the tuned frequency that produces the same indication on the measuring receiver shall be not less than 40 dB. Examples of the frequencies from which such spurious responses may occur are as follows:

$$(1/m) (nf_L \pm f_i) \text{ and } (1/k) (f_o)$$

where

m, n, k are integers;

f_L is the local oscillator frequency;

f_i is the intermediate frequency;


f_o is the tuned frequency.

NOTE Where more than one intermediate frequency is used, the frequencies f_L and f_i may refer to each of the local oscillator and intermediate frequencies used. In addition, spurious responses may occur when no input signal is applied to the measuring receiver; for example, when harmonics of the local oscillators differ in frequency by one of the intermediate frequencies. The requirements under this heading therefore cannot apply in these latter cases. The effect of these spurious responses is dealt with in 4.7.2.

4.6 Limitation of intermodulation effects

The response of the measuring receiver shall not be influenced by intermodulation effects when tested as follows.

Arrange the apparatus as shown in figure 3. The pulse generator has a spectrum substantially uniform up to frequency 3) but at least 10 dB down at frequency 4) of the frequencies given in table 4. The band-stop filter has an attenuation at the test frequency of at least 40 dB. Its bandwidth, B_6 , relative to the maximum attenuation of the filter shall lie between the frequencies 1) and 2) given in table 4.

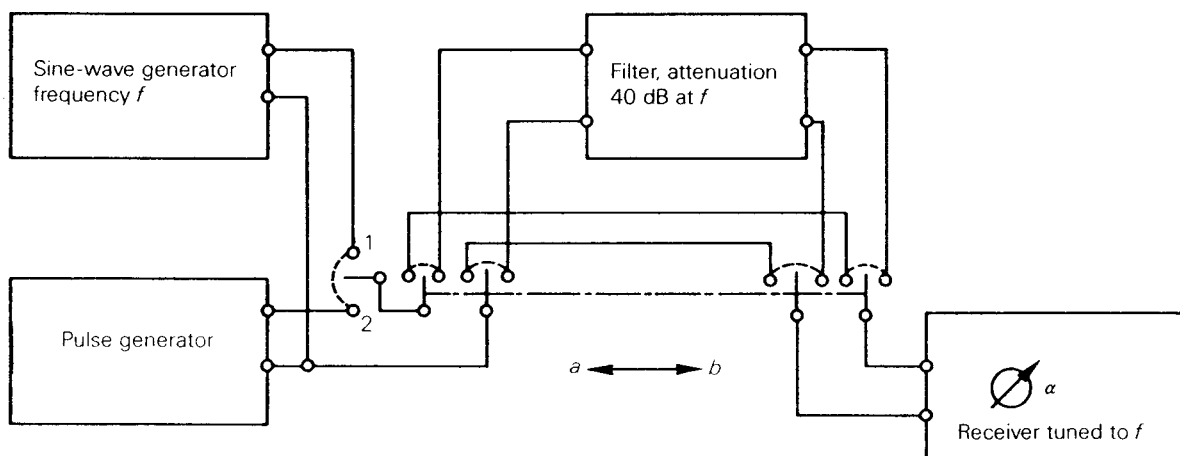

IEC 1297/99

Responses:

$$\alpha_{1a} = \alpha_{2a}$$

$$\alpha_{1b} = \alpha_{1a} - 40 \text{ dB}$$

$$\alpha_{2b} = \alpha_{2a} - 36 \text{ dB}$$

Figure 3 – Arrangement for testing intermodulation effects

Table 4 – Bandwidth characteristics for inter-modulation test of quasi-peak measuring receivers

Frequency range	1) kHz	2) kHz	3) MHz	4) MHz
9 kHz to 150 kHz (band A)	0,4	4	0,15	0,3
0,15 MHz to 30 MHz (band B)	20	200	30	60
30 MHz to 300 MHz (band C)	500	2 000	300	600
300 MHz to 1 000 MHz (band D)	500	6 000	1 000	2 000

Connect the sine-wave generator output direct to the measuring receiver input and adjust for a convenient reading. Substitute the pulse generator for the sine-wave generator and adjust for the same reading. The pulse repetition frequency shall be 100 Hz for band A and 1 000 Hz for the other bands.

With the pulse generator connected as described above, switching the filter into circuit shall introduce attenuation of not less than 36 dB.

4.7 Limitation of receiver noise and internally generated spurious signals

4.7.1 Random noise

The background noise shall not introduce an error in excess of 1 dB.

NOTE For a measuring apparatus incorporating attenuation in the intermediate frequency amplifier, this condition will be regarded as being satisfied if the apparatus complies with the following test:

A sine-wave signal is applied to the input of the measuring apparatus and adjusted to a value S_1 , such that the output meter shows a reference deflection θ . An attenuation of 10 dB is introduced in the intermediate-frequency stages. The level of the input signal is increased to S_2 so as to restore the output meter to the deflection θ . The increase of the level of the input signal ($S_2 - S_1$) shall be between 10 dB and 11 dB.

4.7.2 Continuous wave

Where more than one intermediate frequency is used, the existence of spurious responses as described in the note to 4.5.4 shall not introduce a measurement error in excess of 1 dB for any signal input to the measuring receiver. For a measuring receiver incorporating attenuation in the i.f. amplifier, this requirement shall be regarded as satisfied if the receiver complies with 4.7.1 when tested as described in 4.7.1, except that the attenuation in the intermediate stages shall be introduced after the last mixer stage.

4.8 Screening effectiveness

Screening effectiveness is a measure of the ability of the measuring receiver to operate in an electromagnetic field without degradation. The requirement applies to receivers operating within the "CISPR indication range" specified by the manufacturer as described in 3.9.

The screening of the receiver shall be such that when it is immersed in an ambient electromagnetic field of 3 V/m (unmodulated) at any frequency in the range 9 kHz to 1 000 MHz, an error of not greater than 1 dB is produced at the maximum and minimum of the CISPR indicating range as specified by the manufacturer of the receiver. In cases where a measuring receiver is not immune to the requirement of 3 V/m, the field strength and frequency at which the error exceeds 1 dB shall be stated by the manufacturer. The test shall be performed as described below.

The receiver is placed inside a screened enclosure. An input signal is applied to the receiver via a 2 m long well-screened cable (e.g. semi-rigid), through a feedthrough in the enclosure wall, to a signal generator placed outside the enclosure. The level of the input signal shall be at the maximum and the minimum of the CISPR indication range as specified by the manufacturer of the receiver. All other coaxial terminals of the receiver shall be terminated in their characteristic impedance.

Only essential leads (e.g. mains and input cables) for the normal use of the measuring receiver in its minimum configuration (excluding options such as headphones) shall be connected during the test. The leads shall have the lengths and be arranged as in typical use.

The strength of the ambient field in the vicinity of the measuring receiver shall be measured by a field strength monitor.

The receiver meter indication in the presence of the ambient electromagnetic field shall differ by not more than 1 dB from the meter indication when the field is absent.

4.8.1 Limitation of radio-frequency emissions from the measuring receiver

4.8.1.1 Conducted emissions

The radio disturbance voltage at any connecting pin of external lines (not only the mains terminals) shall not exceed the limits for class B equipment given in 5.1 of CISPR 11. The measurement of the radio disturbance voltage is however not required on the inner conductors of screened connections to screened equipment. The local oscillator injection power at the measuring receiver input terminated with its characteristic impedance shall not exceed 34 dB(pW) which is equivalent to 50 μ V across 50 Ω .

4.8.1.2 Radiated emissions

The radio disturbance field strength emitted by the measuring receiver shall not exceed the limits for class B equipment given in 5.2 of CISPR 11, for the frequency range of 9 kHz to 1 000 MHz. The limits shall also apply for frequency bands (ISM frequencies) listed in table 1 of the same publication. In the frequency range of 1 GHz to 18 GHz, a limit of 45 dB(pW) shall apply.

Before performing radiated and conducted emission measurements, it is essential that the noise contributions of the test equipment do not affect the measured results (e.g. computer control).

4.9 Facilities for connection to a discontinuous disturbance analyzer

For all bands the disturbance measuring receiver shall have both an intermediate-frequency output and an output from the quasi-peak detector for the measurement of discontinuous disturbance. The loading of these outputs shall have no influence on the indicating instrument.

5 Peak measuring receivers for the frequency range 9 kHz to 1 000 MHz

This clause specifies requirements for measuring receivers employing a peak detector when used for the measurement of impulsive disturbance.

5.1 Input impedance

The input circuit of measuring receivers shall be unbalanced. For receiver control settings within the CISPR indicating range, the input impedance shall be nominally 50 Ω with a VSWR not to exceed 2,0 to 1 when the RF attenuation is 0 and 1,2 to 1 when the RF attenuation is 10 dB or greater.

Symmetric input impedance in the frequency range 9 kHz to 30 MHz: To permit symmetric measurements a balanced input transformer is used. The preferred input impedance is 600 Ω for the frequency range 9 kHz to 150 kHz. This symmetric input impedance may be incorporated either in the relevant symmetrical artificial network necessary to couple to the receiver or optionally in the measuring receiver.

5.2 Fundamental characteristics

5.2.1 Bandwidth

For all types of broadband disturbance except non-overlapping disturbance, the actual value of the bandwidth shall be stated when the disturbance level is quoted and the bandwidth at the 6 dB points shall lie within the values in table 5.

Table 5 – Bandwidth requirements

Frequency range	Bandwidth B_6	Preferred BW
9 kHz to 150 kHz (band A)	100 Hz to 300 Hz	200 Hz
0,15 MHz to 30 MHz (band B)	8 kHz to 10 kHz	9 kHz
30 MHz to 300 MHz (bands C and D)	100 kHz to 500 kHz	120 kHz
NOTE Since the response of a peak measuring receiver to non-overlapping pulses is proportional to its impulse bandwidth, either the actual bandwidth is quoted in the result or the level may be quoted as that "in a 1 MHz bandwidth" calculated by dividing the measured value by the impulse bandwidth in MHz (see 3.2). For other types of broadband disturbance this procedure would introduce an error.		

5.2.2 Charge and discharge time constants ratio

In order to achieve a meter reading within 10 % of the true value of the peak at a repetition rate of 1 Hz, the discharge time constant to charge time constant ratio shall be not less than the values given below.

- $1,89 \times 10^4$ in the frequency range 9 kHz to 150 kHz;
- $1,25 \times 10^6$ in the frequency range 150 kHz to 30 MHz;
- $1,67 \times 10^7$ in the frequency range 30 MHz to 1 000 MHz.

If a peak-hold facility is incorporated, the hold time shall be capable of being set to values between 30 ms and 3 s.

NOTE Care should be taken to ensure that any recording instrument used is capable of full response within the selected hold time.

5.2.3 Overload factor

For peak measuring receivers, the overload factor need not be so great as for other types of measuring receiver. For most direct-reading detectors, the overload factor need be only a little greater than unity. The overload factor shall be adequate for the time-constants used (see 5.2.2).

5.3 Sine-wave voltage accuracy

The accuracy of measurement of sine-wave voltages shall be better than ± 2 dB when supplied with a sine-wave signal at a 50Ω resistive source impedance.

5.4 Response to pulses

The response of the measuring receiver to pulses of impulse area $1,4/B_{\text{imp}}$ mVs (where B_{imp} is in hertz) e.m.f. at 50Ω source impedance shall be equal to the response to an unmodulated sine-wave signal at the tuned frequency having an e.m.f. of r.m.s. value 2 mV (66 dB(μ V)). The source impedances of the pulse generator and the signal generator shall both be the same. The pulses shall have a uniform spectrum according to table 2 of 4.4.1.

A tolerance of $\pm 1,5$ dB is permitted in the sine-wave voltage level and this requirement applies for all pulse repetition frequencies for which no overlapping pulses occur at the output of the i.f. amplifier.

NOTE 1 Annexes B and C describe methods for determining the output characteristics of pulse generators for use in testing the requirements of this subclause.

NOTE 2 At a repetition rate of 25 Hz for band A and 100 Hz for the other bands, the relationship between the indications of a peak measuring receiver and a quasi-peak measuring receiver with the preferred bandwidth are given in table 6.

Table 6 – Relative pulse response of peak and quasi-peak measuring receivers for the same bandwidth

Frequency	IS mVs	B_{imp} Hz	Ratio peak/quasi-peak (dB) for pulse repetition rate	
			25 Hz	100 Hz
Band A	$6,67 \times 10^{-3}$	$0,21 \times 10^3$	6,1	–
Band B	$0,148 \times 10^{-3}$	$9,45 \times 10^3$	–	6,6
Bands C and D	$0,011 \times 10^{-3}$	$126,0 \times 10^3$	–	12,0

5.5 Selectivity

Since the bandwidth requirements of 5.2.1 allow variations from the bandwidths given in figures 2a, 2b and 2c, these selectivity curves apply to peak measuring receivers as regards shape only, and the frequency axis shall be scaled accordingly. For example, $B_6/2$ corresponds to 100 Hz in figure 2a.

The requirements of 4.5.2, 4.5.3 and 4.5.4 apply.

5.6 Intermodulation effects, receiver noise, and screening

The requirements of 4.6, 4.7 and 4.8 apply.

6 Average measuring receivers for the frequency range 9 kHz to 1 000 MHz

This type of receiver has a detector designed to indicate the average value of the envelope of the signal passed through the pre-detector stages. The average detector is used for the measurement of narrowband signals to overcome problems associated with either modulation content or the presence of broadband noise. Average measuring receivers are not generally used for the measurement of impulsive disturbance.

6.1 Input impedance

The input circuit of measuring receivers shall be unbalanced. For receiver control settings within the CISPR indicating range, the input impedance shall be nominally 50 Ω with a VSWR not to exceed 2,0 to 1 when the RF attenuation is 0 and 1,2 to 1 when the RF attenuation is 10 dB or greater.

Symmetric input impedance in the frequency range 9 kHz to 150 kHz: To permit symmetrical measurements a balanced input transformer is used. The preferred input impedance for the frequency range 9 kHz to 150 kHz is 600 Ω . This symmetric input impedance may be incorporated either in the relevant symmetrical artificial network necessary to couple to the receiver or optionally in the measuring receiver.

6.2 Fundamental characteristics

6.2.1 Bandwidth

The bandwidths B_6 shall lie within the values in table 7:

Table 7 – Bandwidth requirements

Frequency range	Bandwidth B_6	Preferred BW
9 kHz to 150 kHz (band A)	100 Hz to 300 Hz	200 Hz
150 kHz to 30 MHz (band B)	8 kHz to 10 kHz	9 kHz
30 MHz to 1 000 MHz (bands C and D)	100 kHz to 500 kHz	120 kHz
NOTE The subject of bandwidth is discussed in annex E, clause E.1. If a bandwidth other than the preferred one is used, it shall be stated when the disturbance level is quoted.		

6.2.2 Overload factor

The overload factor for circuits preceding the detector at a pulse repetition rate of n Hz shall be B_{imp}/n , with B_{imp} in Hz.

The receiver shall not overload for pulse rates equal to or greater than 25 Hz for band A, 500 Hz for band B, and 5 000 Hz for bands C and D.

NOTE With this type of receiver it will not, in general, be possible to provide a sufficient overload factor to prevent non-linear operation of the receiver at very low pulse rates (the response to a single pulse is not defined).

6.3 Sine-wave voltage accuracy

The accuracy of measurement of sine-wave voltages shall be better than ± 2 dB when supplied with a sine-wave signal at 50 Ω resistive source impedance.

6.4 Response to pulses

NOTE – Annexes B and C describe methods for determining the output characteristics of pulse generators for use in testing the requirements of this clause.

6.4.1 Amplitude relationship

The response of the measuring receiver to pulses of repetition rate n Hz and impulse area e.m.f. at 50 Ω source impedance equal to $1,4/n$ mVs, shall be equal to the response to an unmodulated sine-wave signal at the tuned frequency having an e.m.f. of r.m.s. value 2 mV (66 dB(μ V)). The source impedances of the pulse generator and the signal generator shall both be the same. The pulses shall have a uniform spectrum according to table 2 of 4.4.1. The value of n shall be 25 for band A, 500 for band B, and 5 000 for bands C and D. A tolerance of 2,5 dB/–0,5 dB is permitted on the sine-wave voltage level.

NOTE 1 A lower impulse area may be used together with a proportionally lower amplitude for the unmodulated sine-wave input, provided sufficient signal-to-noise ratio is maintained.

NOTE 2 At repetition frequencies of 25, 100, 1 000 and 10 000 Hz, the relationship between the indications of an average and a quasi-peak measuring receiver of the same bandwidth, assuming adequate overload factors and a constant output level, is given in table 8.

Table 8 – Relative pulse response of average and quasi-peak measuring receivers for the same bandwidth

Frequency range of measuring receiver	Ratio quasi-peak/average indications (dB) for pulse repetition rate				
	25 Hz	100 Hz	500 Hz	1 000 Hz	5 000 Hz
9 kHz to 150 kHz (band A)	12,4				
0,15 MHz to 30 MHz (band B)		(32,9)	22,9	(17,4)	
30 MHz to 1 000 MHz (bands C/D)				(38,1)	26,3
NOTE Values in brackets are for information only.					

6.4.2 Variation with repetition frequency

The response of the measuring receiver to repeated pulses shall be such that, for a constant indication on the measuring receiver, the relationship between amplitude and repetition frequency is in accordance with the following law.

Amplitude proportional to (repetition frequency)^{–1}

A tolerance of +3 dB to –1 dB is permitted in the frequency range from the lowest repetition frequency usable as determined from overload considerations to a frequency equal to $B_3/2$.

NOTE The theoretical pulse response curves of quasi-peak and average detector receivers, combined on an absolute scale, are shown in figure 1d.

6.4.3 Response to intermittent, unsteady and drifting narrowband disturbances

The response to intermittent, unsteady and drifting narrowband disturbances shall be such that the measurement result is equivalent to the peak reading of a meter with a time constant of 160 ms for bands A and B and of 100 ms for bands C and D, as depicted in Figure 5. The time constant is as defined in A.3.1. This can be accomplished by a meter simulating network following the envelope detector of the receiver. The peak reading may be taken, for example,

by continuous monitoring of the meter output using an A/D converter and a microprocessor, as shown in Figure 4.


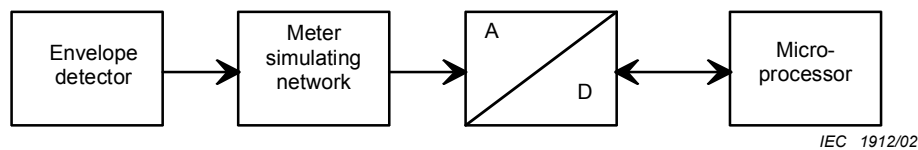


Figure 4 – Block diagram of an average detector

It is deduced from the above requirement that an average measuring receiver shall yield the maximum reading listed in table 9 for a radiofrequency sine-wave input signal modulated with repeated rectangular pulses having the duration and period indicated in the table. A tolerance of $\pm 1,0$ dB is allowed for this requirement.

Table 9 – Maximum reading of average measuring receivers for a pulse-modulated sine-wave input in comparison with the response to a continuous sine-wave having the same amplitude

Repeated rectangular pulses for modulation	Band A/B receiver $T_M = 0,16$ s	Band C/D receiver $T_M = 0,1$ s
Duration = T_M Period = 1,6 s	0,353 (= -9,0 dB)	0,353 (= -9,0 dB)

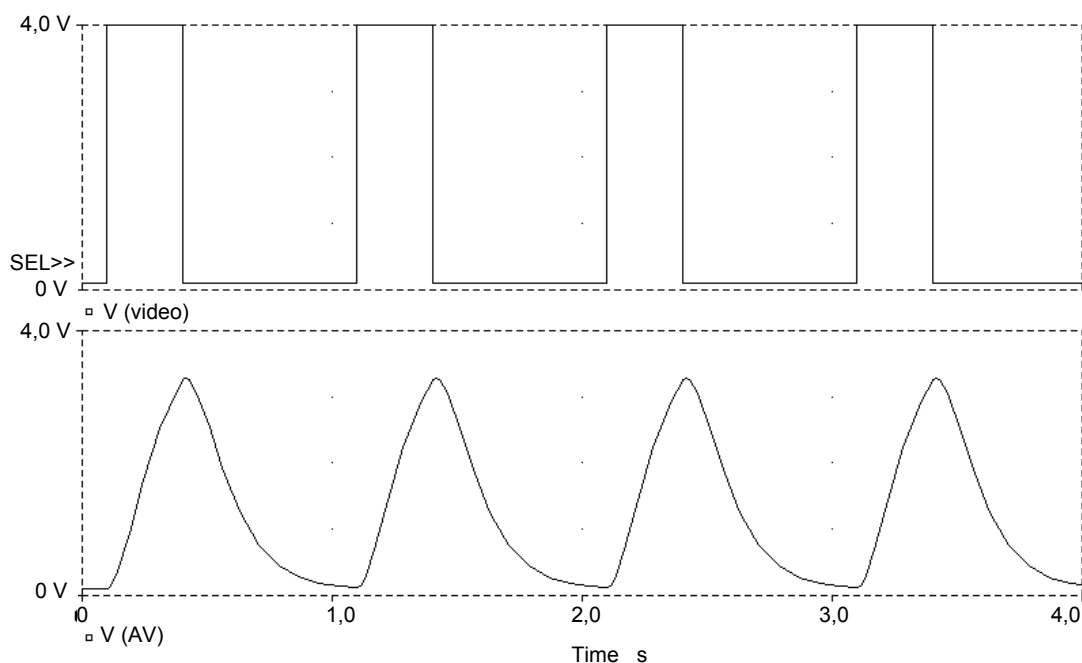

NOTE The response shown is caused by an intermittent narrowband signal with a duration of 0,3 s and a repetition frequency of 1 Hz, when a time constant of 100 ms is used. If the time constant is 160 ms, the peaks at the output of the meter simulating network will be lower.

Figure 5 – Response of the meter simulating network to an intermittent narrowband signal

6.5 Selectivity

For receivers with a bandwidth of 200 Hz (for frequency range 9 kHz to 150 kHz) or a bandwidth of 9 kHz (for frequency range 0,15 MHz to 30 MHz) the overall selectivity shall be within the limits shown in figures 2a and 2b, respectively. For receivers with a bandwidth of 120 kHz (for frequency range 30 MHz to 1 000 MHz), the overall selectivity shall be within the limits shown in figure 2c. For receivers having other bandwidths, the figures 2a, 2b and 2c describe the shape only, and the frequency axis shall be scaled accordingly.

The requirements of 4.5.2, 4.5.3 and 4.5.4 apply.

NOTE – For the measurement of equipment that requires higher selectivity at the transition between 130 kHz and 150 kHz (e.g. mains signalling equipment as defined in EN 50065-1/A2), a highpass filter may be added in front of the measuring receiver to achieve the following combined selectivity of CISPR measuring receiver and highpass filter:

Frequency kHz	Relative attenuation dB
150	≤ 1
146	≤ 6
145	≥ 6
140	≥ 34
130	≥ 81

The measuring receiver in conjunction with the highpass filter should fulfil the requirements of this standard.

6.6 Intermodulation effects, receiver noise, and screening

The requirements of 4.6, 4.7 and 4.8 apply.

7 RMS measuring receivers for the frequency range 9 kHz to 1 000 MHz

7.1 Input impedance

The input circuit of measuring receivers shall be unbalanced. For receiver control settings within the CISPR indicating range, the input impedance shall be nominally 50 Ω with a VSWR not to exceed 2,0 to 1 when the RF attenuation is nil and 1,2 to 1 when the RF attenuator is 10 dB or greater.

Symmetric input impedance in the frequency range 9 kHz to 30 MHz: To permit symmetrical measurements a balanced input transformer is used. The preferred input impedance for the frequency range 9 kHz to 150 kHz is 600 Ω . This symmetric input impedance may be incorporated either in the relevant symmetrical artificial network necessary to couple to the receiver or optionally in the measuring receiver.

7.2 Fundamental characteristics

7.2.1 Bandwidth

Since the response of an r.m.s. meter is proportional to the square root of the bandwidth for any type of broadband disturbance, the actual bandwidth need not be specified. For such broadband disturbance, the measurement result may be quoted as that "in 1 kHz bandwidth", by dividing the measured value by the square root of the power bandwidth given in kilohertz. The actual value of the bandwidth shall be stated when the disturbance level is quoted.

7.2.2 Overload factor

The overload factor for circuits preceding the detector at a pulse repetition rate of n Hz shall be $1,27(B_3/n)^{1/2}$, with B_3 in Hz.

NOTE 1 With this type of detector it will not, in general, be possible to provide a sufficient overload factor to prevent non-linear operation of the instrument at very low pulse repetition rates (the response to a single pulse is not defined). In any application of this detector, the minimum pulse repetition rate without overload shall be determined.

NOTE 2 Annex A describes the calculation for the overload factor.

7.3 Sine-wave voltage accuracy

The accuracy of measurement of sine-wave voltages shall be better than ± 2 dB when supplied with a sine-wave signal at 50Ω resistive source impedance.

7.4 Response to pulses

NOTE Annexes B and C describe methods for determining the output characteristics of pulse generators for use in testing the requirements of this clause.

7.4.1 Amplitude relationship

The response of the measuring receiver for band A to pulses of impulse area $[278 (B_3)^{-1/2}] \mu\text{Vs}$ e.m.f. (with B_3 in Hz) at 50Ω source impedance having a uniform spectrum up to at least the highest tuneable frequency of the receiver, repeated at a frequency of 25 Hz shall, for all frequencies of tuning, be equal to the response to an unmodulated sine-wave signal at the tuned frequency having an e.m.f. of 2 mV (66 dB(μV)) r.m.s. For the measuring receivers for bands B, C and D, the corresponding values are $[139 (B_3^{-1/2})] \mu\text{Vs}$ (with B_3 in Hz) and 100 Hz. The source impedances of the pulse generator and the signal generator shall both be the same. A tolerance of $\pm 1,5$ dB is permitted in the sine-wave voltage levels prescribed above.

NOTE 1 Annex A describes the calculation for the pulse response of the r.m.s. detector. At a repetition frequency of 25 Hz and 100 Hz, respectively, the relationship between the indications of an r.m.s. and a quasi-peak measuring receiver of the same bandwidth is given in table 10.

NOTE 2 A lower impulse area may be used together with a proportionally lower amplitude for the unmodulated sine-wave input, provided sufficient signal-to-noise ratio is maintained.

Table 10 – Relative pulse response of r.m.s. and quasi-peak measuring receivers

Frequency range of measuring receiver	Pulse repetition range	Ratio quasi-peak/r.m.s. indications
	Hz	dB
9 kHz to 150 kHz (band A)	25	4,2
0,15 MHz to 30 MHz (band B)	100	14,3
30 MHz to 1 000 MHz (bands C and D)	100	20,1

7.4.2 Variation with repetition frequency

The response of the measuring receiver to repeated pulses shall be such that, for a constant indication on the measuring receiver, the relationship between amplitude and repetition frequency shall be in accordance with the following law:

Amplitude proportional to (repetition frequency) $^{-1/2}$

The response curve for a particular receiver shall lie between the limits in table 11.

Table 11 – Pulse response of r.m.s. receiver

Repetition frequency Hz	Relative equivalent level of pulse dB	
	Band A	Bands B, C and D
1 000	–	$-10 \pm 1,0$
100	$-6 \pm 0,6$	0 (ref.)
25	0 (ref.)	$+6 \pm 0,6$
20	$+1 \pm 0,7$	$+7 \pm 0,7$
10	$+4 \pm 1,0$	$+10 \pm 1,0$
2	$+11 \pm 1,7$	$+17 \pm 1,7$
1	$+14 \pm 2,0$	$+20 \pm 2,0$

7.5 Selectivity

Since the bandwidth requirements of 7.2.1 allow variations from the bandwidths given in figures 2a, 2b and 2c, these selectivity curves apply to r.m.s. measuring receivers as regards shape only, and the frequency axis shall be scaled accordingly. For example, $B_6/2$ corresponds to 100 Hz in figure 2a.

The requirements of 4.5.2, 4.5.3 and 4.5.4 apply.

7.6 Intermodulation effects, receiver noise, and screening

The requirements of 4.6, 4.7 and 4.8 apply.

8 Spectrum analyzers and scanning receivers

8.1 Spectrum analyzers and scanning receivers for the frequency range 9 kHz to 1 000 MHz

Spectrum analyzers and scanning receivers intended for the measurement of disturbance in the frequency range 9 kHz to 1 000 MHz shall comply with the performance requirements specified in clauses 4, 5 or 6.

8.2 Spectrum analyzers and scanning receivers for the frequency range 1 GHz to 18 GHz

The spectrum analyzer is the most commonly used equipment for measurements above 1 GHz. The measurement method in this range is based on this equipment. The use of measuring receivers with stepped frequency scanning is however not excluded. The indications below apply, as appropriate.

Requirements for measuring apparatus in the frequency range 1 GHz to 18 GHz are listed below:

a) Resolution bandwidth (RBW)

For general measurements above 1 GHz, the resolution bandwidth (RBW) of the measuring receiver shall be 1 MHz. In justified cases, depending on the system to be protected, the source and the emission limit, narrower or wider RBW may be specified by the relevant product committee.

The chosen value shall be defined with a tolerance of $\pm 10\%$ (1 MHz $\pm 10\%$ for example). This RBW shall be defined as the impulse bandwidth of the measuring apparatus.

b) Detector

The peak detector is a standard detector on spectrum analyzers and is therefore the preferred detector for emission measurements above 1 GHz. A maximum hold function may be used for signals varying with time.

Additional measurements with a weighting detector may also be applicable to some products or product families if it is appropriate to evaluate its interfering potential towards radio systems. A weighting function can be achieved by reducing the video bandwidth of the spectrum analyzer.

NOTE – For weighted measurements based on a reduction of the video bandwidth, care should be taken that the scanning time is sufficiently long to allow the video filter to respond in a correct way.

c) Video bandwidth (VBW)

For measurements with a peak detector, the VBW shall be higher than the RBW (1 MHz, see 8.2 a)). On generally available measuring equipment, this corresponds to a VBW set to three times the RBW.

To reach weighted measurements, the VBW should be set to a value lower than the modulation bandwidth of the signal to be measured. The evaluation of the correct VBW can be done by reducing the VBW until the indicated amplitude changes by less than approximately 1 dB. Linearity reserve requirements for the stages preceding the detector are under consideration.

NOTE For peak measurements, the output signal of the peak detector can be read from the display operating in either the linear or the logarithmic mode. For weighted measurements, if the linear mode is used, the result will correspond to the average level of the measured signal; if the logarithmic mode is used, the result will correspond to the average of the logarithmic values of the measured signal. Thus, for a square signal taking alternatively the values 20 dB(μ V) and 60 dB(μ V), the level obtained in the logarithmic mode is 40 dB(μ V), whereas in the linear mode, the level of 54,1 dB(μ V) represents the true average value of the signal.

d) Screening effectiveness

For the frequency range of 1 GHz to 18 GHz, the screening effectiveness is under consideration.

e) Input filter

A filter shall be provided at the input of the spectrum analyzer to give sufficient attenuation at the fundamental frequency of certain equipment under test to protect the input circuits of the analyzer from overload and damage and to prevent the generation of harmonic and intermodulation signals when measuring weak spurious signals in the presence of a strong fundamental signal.

NOTE 1 30 dB filter attenuation at the fundamental frequency of the equipment under test is normally adequate.

NOTE 2 A number of such filters may be required to deal with more than one fundamental frequency.

f) Display

To permit visual observations while using the slower sweep times, the spectrum analyzer shall be provided with some form of display storage.

g) Scanning time

The scan time for the displayed frequency range should be capable of being varied, e.g., from 0,1 s to 10 s.


NOTE The definition of additional parameters of the measuring apparatus such as input impedance, linearity, sine-wave voltage accuracy, absolute calibration, etc. is presently under consideration.

9 Audio-frequency voltmeter

In the CISPR, a voltmeter is needed which can be utilized for checking purposes, which when connected to the output of a good radio receiver will give significant measurements compared with a standard CISPR quasi-peak measuring receiver. It should be noted, however, that the use of the meter in this manner as compared to a normal CISPR receiver will be limited in performance by the bandwidth, overload, non-linearity and spurious responses of the radio receiver. The IEC has prepared specifications* for measuring noise at the audio output of receivers.

The voltmeter also enables assessment to be made of the performance of audio systems subjected to continuous and impulsive noise. It contains various circuits which can be selected depending on the function to be served. Where a specific function is desired, only those circuits necessary for that function need be included.

A block diagram of the voltmeter is shown in figure 6.

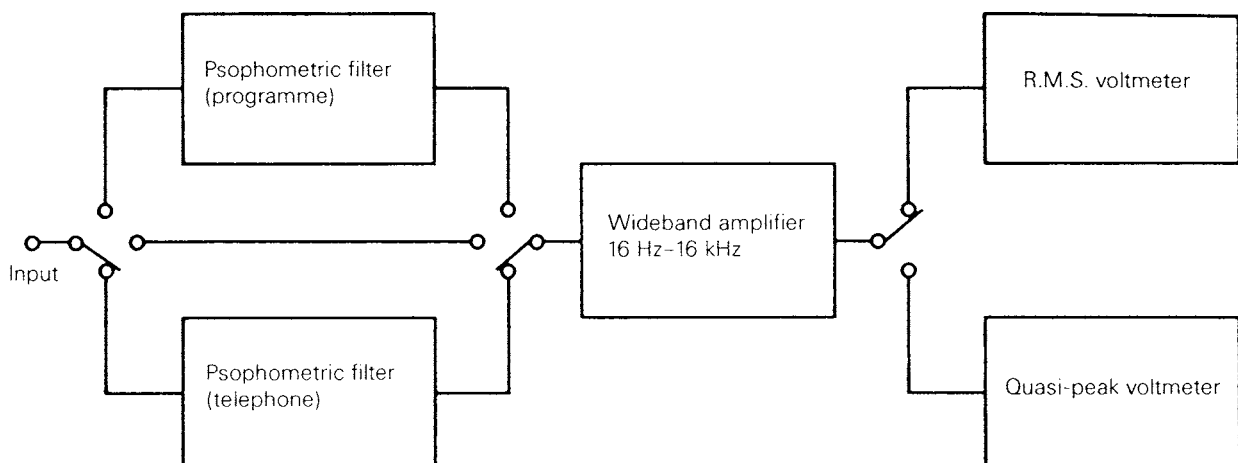

IEC 1298/99

Figure 6 – Block diagram of an audio-frequency interference voltmeter

9.1 Fundamental characteristics

9.1.1 Input impedance

The rated input impedance shall be one or more of the following values, unbalanced, 50 Ω and a high impedance not less than 6 000 Ω , and balanced, 600 Ω .

The balance of the 600 Ω input shall be such that when a voltage U is applied between the voltmeter ground and the mid-point of a 600 Ω resistor connected across the input terminals, the output indication shall not exceed 0,1 mV. The value of the voltage U for the test shall be in accordance with table 12:

* IEC 60315-3 for a.m. receivers.
IEC 60315-4 for f.m. receivers.

Table 12 – Balance requirement

Frequency Hz	Asymmetrical input voltage for 0,1 mV symmetrical output voltage U (V)	Common mode rejection dB
50	200	126
250	40	112
1 000	10	100

9.1.2 Sensitivity

The measuring range of the voltmeter for an input frequency of 1 kHz shall cover 0,3 mV full scale to 1 V full scale.

9.1.3 Frequency response

The response of the components of the voltmeter to sine-wave input signals shall be as follows:

- a) frequency response of the wideband amplifier: 3 dB at 16 Hz and 16 kHz
- b) telephone psophometric filter: see figure 7**
- c) sound programme psophometric filter: see figure 8***

9.2 Sine-wave voltage accuracy

The accuracy of measurement of sine-wave voltages shall be better than ± 2 dB when supplied with a sine-wave signal at 50 Ω resistive source impedance.

9.3 Screening

The screening of the meter shall be such that when it is immersed in an alternating magnetic field of 1 A/m at the mains supply frequency, an error of not greater than 1 dB is produced at any measuring level.

NOTE Specifications of screening effectiveness to ambient electromagnetic fields are under consideration.

** See CCITT Recommendation P.53, Psophometers (apparatus for the objective measurement of circuit noise). *Blue Book*, Vol. V (1989). See also ITU-R Rec. O.41 (10/94).

*** See ITU-R Recommendation 468-4 (1986).

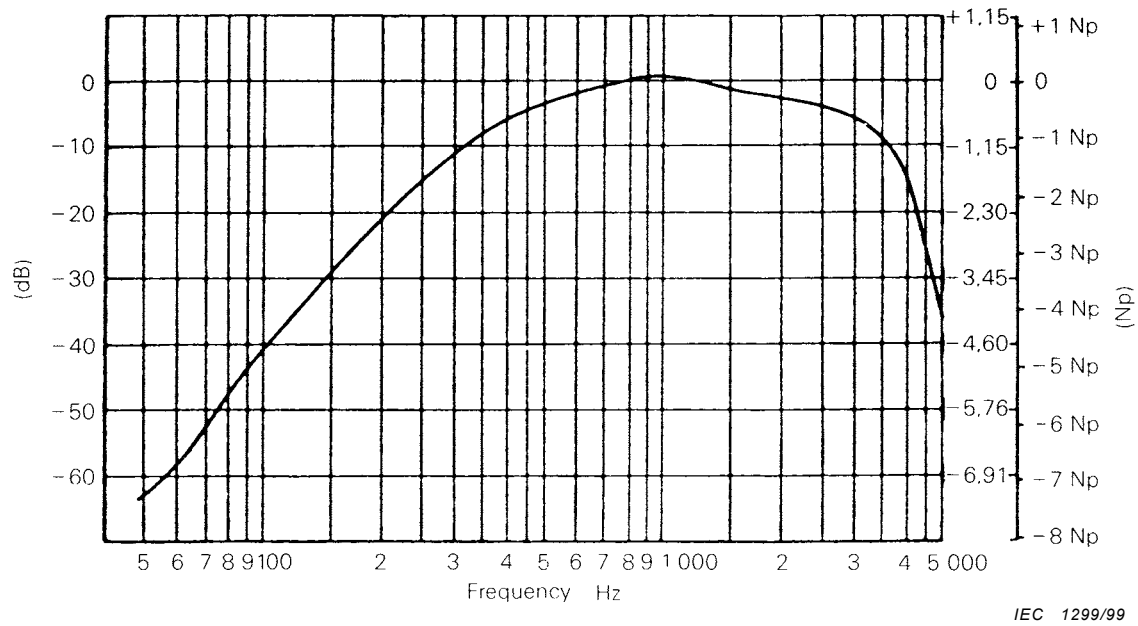


Figure 7 – Characteristic curve of the psophometric filter network used for measurement at the terminals of a commercial trunk telephone circuit

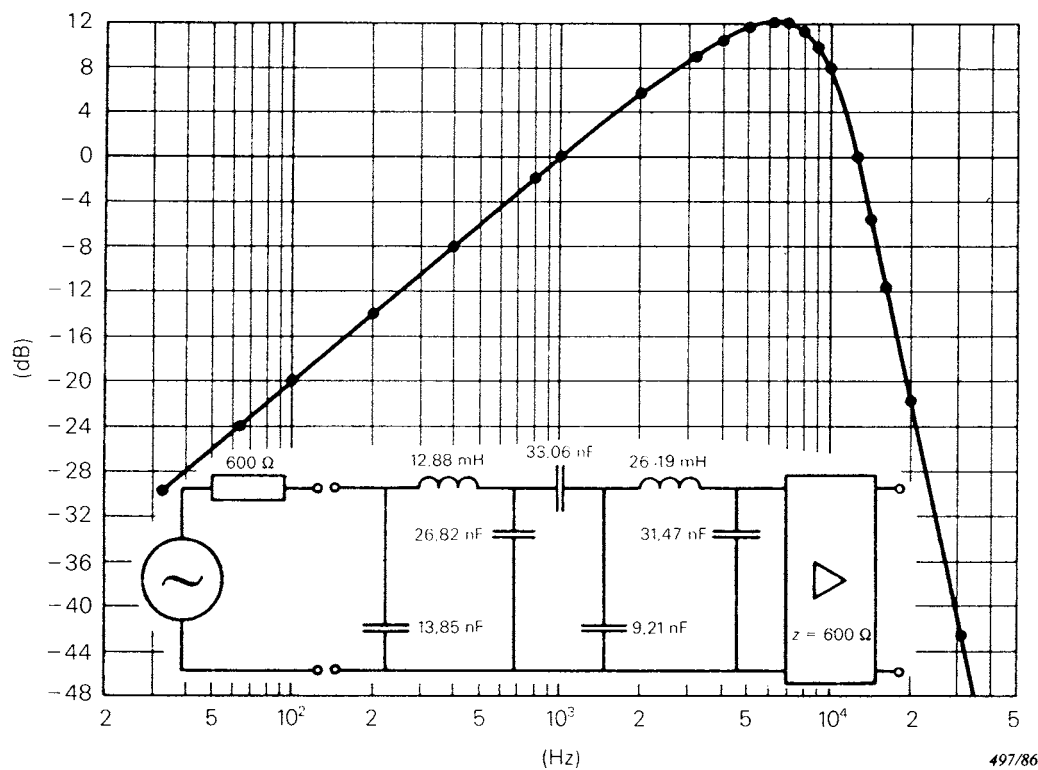


Figure 8 – Weighting network for programme measurement and its response curve

9.4 Requirements for use as a quasi-peak meter

The sound programme psophometric filter shall be used.

9.4.1 Quasi-peak meter fundamental characteristics

The response to pulses as specified in 9.4.2 and 9.4.3 are calculated on the basis of the following nominal fundamental characteristics.

- Overload factor 30 dB
- Charging time constant 1 ms
- Discharging time constant 160 ms
- Mechanical time constant of the critically damped indicating instrument 160 ms

NOTE When used with a measuring receiver, the time constants shall be adjusted to suit the requirements of 9.4.2 and 9.4.3.

9.4.2 Response to pulses

The response to both positive and negative pulses of impulse strength 0,075 μ Vs having a uniform spectrum up to at least 20 kHz, repeated at a frequency of 100 Hz, shall be equal to the response to a 1 000 Hz sine-wave having an e.m.f. of r.m.s. value of 2 mV (66 dB(μ V)). The source impedances of the pulse generator and the sine-wave generator shall be the same. A tolerance of $\pm 1,5$ dB is permitted on the sine-wave voltage level.

9.4.3 Variation with repetition frequency

The response of the meter to repeated pulses shall be such that for a constant indication on the meter, the relationship between amplitude and repetition frequency shall be in accordance with the limits quoted in table 13:

Table 13 – Pulse response requirement

Repetition frequency Hz	Relative equivalent level of pulse dB
1 000	$-4,5 \pm 1,0$
100	0 (reference)
20	$6,5 \pm 1,0$
5	$14,5 \pm 2,0$
Isolated pulse	$23,5 \pm 3,0$

9.5 Requirements for use as an r.m.s. meter

9.5.1 RMS meter fundamental characteristic

The time constant of the electrical circuit of the voltmeter shall be not longer than 1 s.

1.1.2 Response to pulses

For an r.m.s. audio voltmeter with a 3 dB bandwidth B_3 in Hz including the frequency weighting due to the psophometric filter, if any, the response of the meter to pulses of impulse area $139(B_3)^{-1/2}$ μ Vs having a uniform spectrum up to at least 20 kHz, repeated at a frequency of 100 Hz, shall be equal to the response to a sine-wave having an r.m.s. value of 2 mV at the frequency giving the greatest response. The source impedances of the pulse generator and the sine-wave generator shall be the same. A difference of $\pm 1,5$ dB between the two responses is allowed.

9.5.3 Variation with repetition frequency

The response of the voltmeter to repeated pulses shall be such that for a constant indication on the meter, the relationship between amplitude of pulses and repetition frequency shall be in accordance with:

Amplitude proportional to (repetition frequency) $^{-1/2}$

A tolerance of $\pm 1/10$ of the relevant equivalent level of pulse in decibels referred to the level at 100 Hz repetition frequency is allowed.

NOTE The lowest repetition frequency at which it is possible to measure accurately is determined by the overall bandwidth of the voltmeter and a possible receiver (or filter) before it and by the overload factor of the meter (assuming the receiver is not being overloaded). For a low-frequency passband of 9 kHz at 6 dB down and 30 dB overload factor (as for the quasi-peak voltmeter) the lowest repetition frequency is 12 Hz.

10 Disturbance analyzers

Disturbance analyzers are used for the automatic assessment of amplitude, rate and duration of discontinuous disturbances (clicks).

A 'click' has the following characteristics:

- a) the QP amplitude exceeds the quasi-peak limit of continuous disturbance,
- b) the duration is not longer than 200 ms,
- c) and the spacing from a preceding or subsequent disturbance is equal to or more than 200 ms.

A series of short pulses shall be treated as a click when its duration, measured from the start of the first to the end of the last pulse, is not longer than 200 ms and conditions a) and c) are fulfilled.

The time parameters are determined from the signal which exceeds the IF reference level of the measuring receiver.

NOTE 1 Definition and assessment of clicks are in compliance with CISPR 14-1:2000.

NOTE 2 Current analyzers are designed to be used with a quasi-peak measuring receiver of the type which works with a limited internal signal level. As a result, such analyzers may not interface correctly with all receivers.

10.1 Fundamental characteristics

- a) The analyzer shall be equipped with a channel to measure the duration and spacing of discontinuous disturbances; the input of this channel shall be connected to the IF output of the measuring receiver. For these measurements, only the part of the disturbance has to be considered which exceeds the IF reference level of the receiver. The accuracy of duration measurements shall be not worse than ± 5 %.

NOTE 1 The IF reference level is the corresponding value in the IF output of the measuring receiver to an unmodulated sinusoidal signal, which produces a quasi-peak indication equal to the limit for continuous disturbances.


- b) The analyzer shall be equipped with a channel to assess the quasi-peak amplitude of a disturbance.
- c) The amplitude in the quasi-peak channel shall be measured 250 ms after the last falling edge in the IF channel.
- d) The combination of both channels shall comply in all respects with the requirements of 4.1.
- e) The analyzer shall be capable of indicating the following information:
 - the number of clicks of duration equal to or less than 200 ms;
 - the duration of the test in minutes;
 - the click rate;
 - the incidence of disturbances other than clicks which exceed the QP limit of continuous disturbance.

NOTE 2 An example of a disturbance analyzer is shown in form of a block diagram in Figure 9.

- f) For validation of the fundamental characteristics the analyzer has to pass the performance check with all the wave forms (test pulses) in Table 14.









Figure 10 presents in a graphical form the waveforms listed in Table 14.

Figure F.1 presents in a graphical form all the waveforms listed in Table F.1 for the performance check of the exceptions from the definitions of a click according to 4.2.3 of CISPR 14-1.

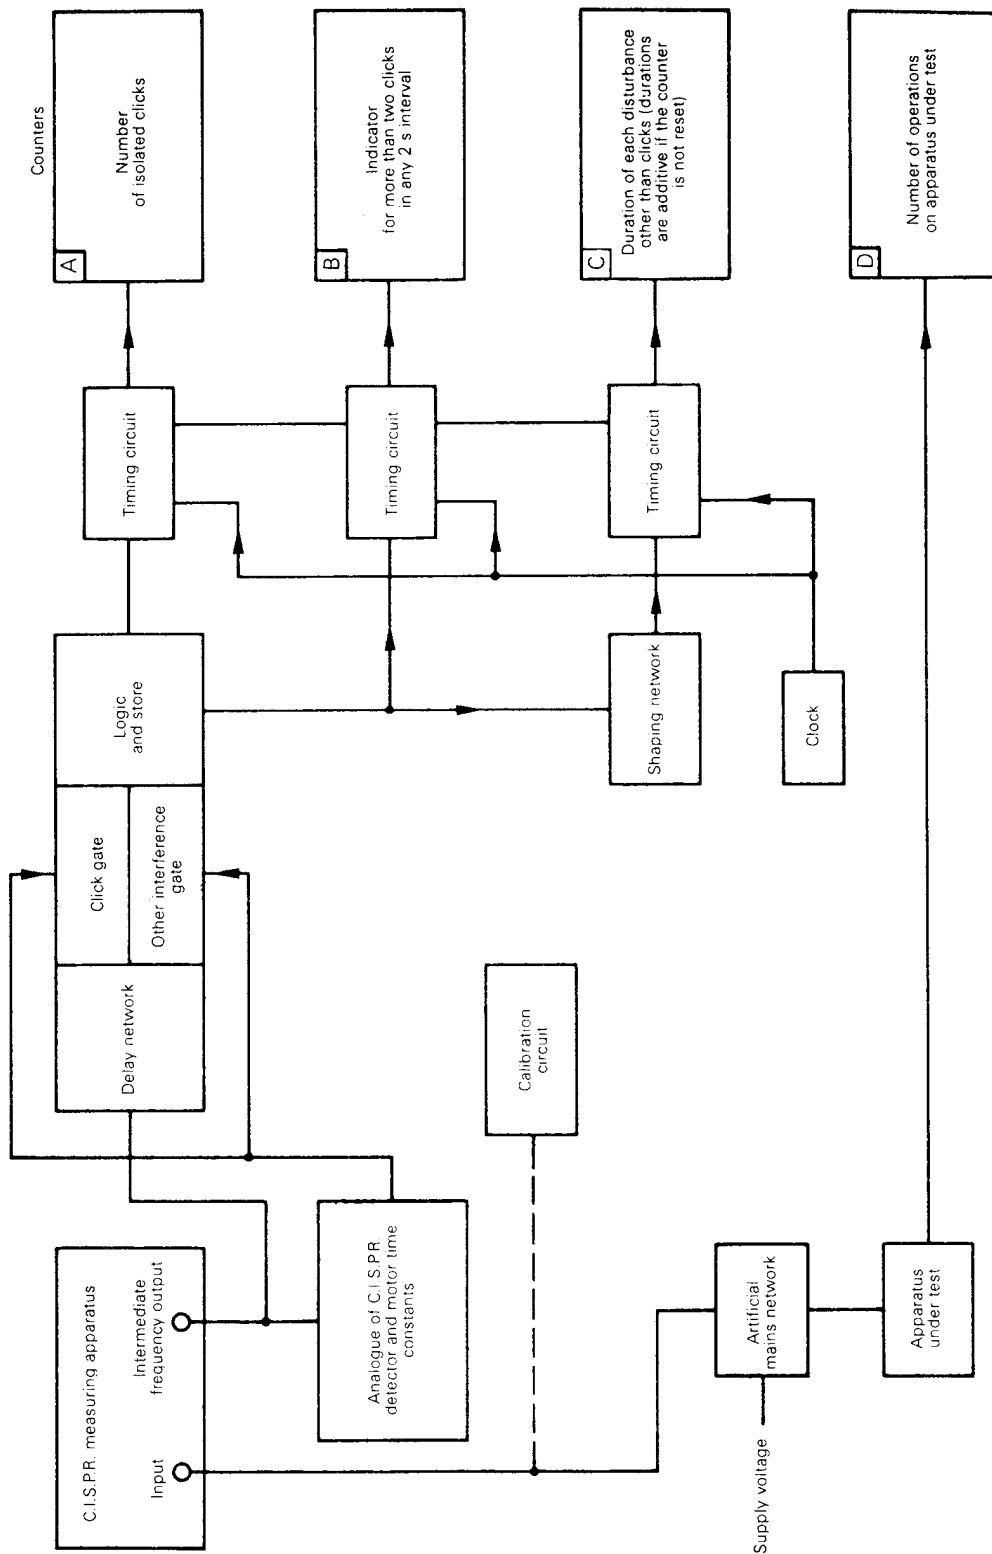

IEC 1305/99

Figure 9 – Example of a disturbance analyzer

Test No.	Test signal	Evaluation by the analyzer
1		1 click
2	 Background: noise or CISPR pulses, 200 Hz: -2,5 dB (QP)	1 click
3	 Background: noise or CISPR pulses, 200 Hz: -2,5 dB (QP)	1 click
4		Other than click
5		Other than click
6		Other than click
7		1 click
8		2 clicks
9	 Min. 21 pulses/0,11 ms/periodicity 10 ms/1 dB	Other than click
10		1 click
11	 Band B: 1034 ms/Band C: under consideration	2 clicks
12	 Band B: 1 166 ms/Band C: under consideration  	1 click

IEC 1115/03

Figure 10 – A graphical presentation of test signals used in the test of the analyzer for the performance check against the definition of a click according to Table 14

**Table 14 – Disturbance analyzer performance test –
Test signals used for the check against the definition of a click**

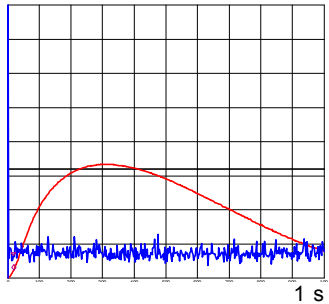
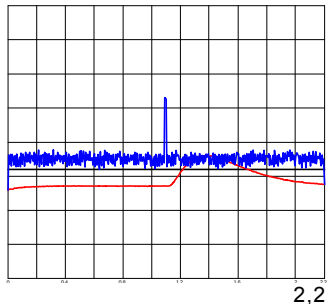
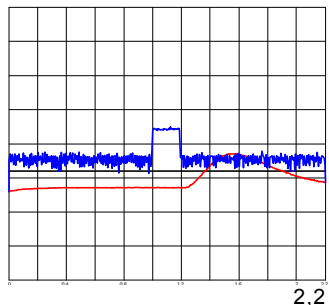
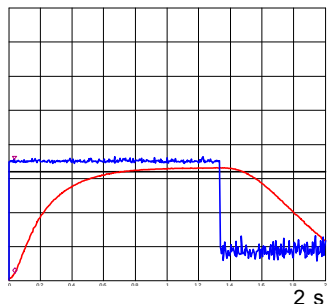
Test No.	Test signal parameters					Evaluation by the analyzer	Graphical presentation of the test signal measured in the IF-output and the associated QP signal relative to the reference indication of the measurement receiver
	1		2		3		
	QP amplitude of impulses adjusted individually relative to QP reference indication of the measurement receiver dB		Duration of impulses ^f adjusted in the intermediate frequency output of the measurement receiver ms		Separation of impulses or periodicity (IF-output) ms		
	Pulse 1	Pulse 2	Pulse 1	Pulse 2			
1	1		0,11			1 click	
2 ^a	1		9,5			1 click	
3 ^a	1		190			1 click	
4	1		1 333 ^b			Other than click	

Table 14 (continued)

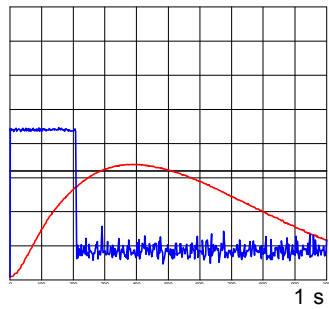
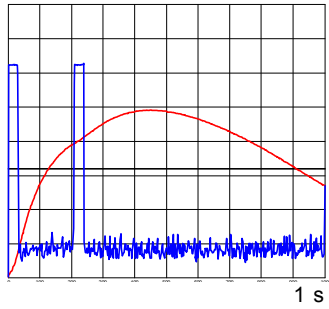
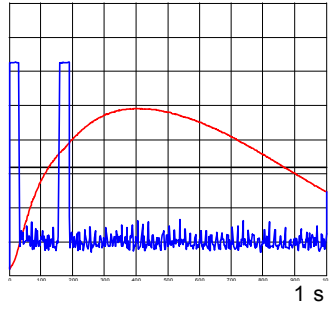
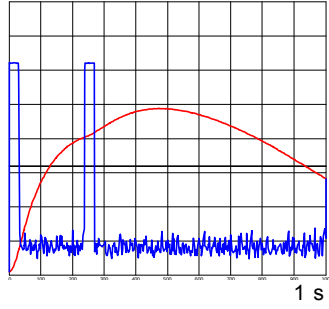
Test No.	Test signal parameters					Evaluation by the analyzer	Graphical presentation of the test signal measured in the IF-output and the associated QP signal relative to the reference indication of the measurement receiver
	1		2		3		
	QP amplitude of impulses adjusted individually relative to QP reference indication of the measurement receiver dB		Duration of impulses ^f adjusted in the intermediate frequency output of the measurement receiver ms		Separation of impulses or periodicity (IF-output) ms		
	Pulse 1	Pulse 2	Pulse 1	Pulse 2			
5	1		210			Other than click (210 ms)	
6	5	5	30	30	180	Other than click (240 ms)	
7	5	5	30	30	130	1 click	
8	5	5	30	30	210	2 clicks	

Table 14 (continued)

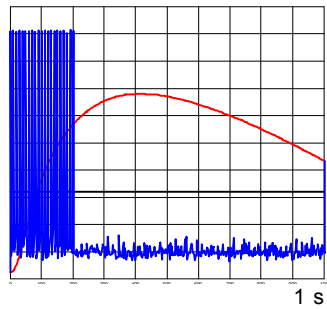
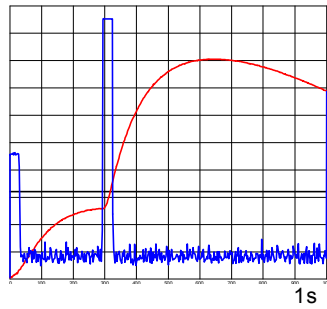
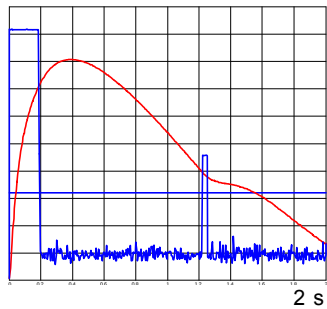
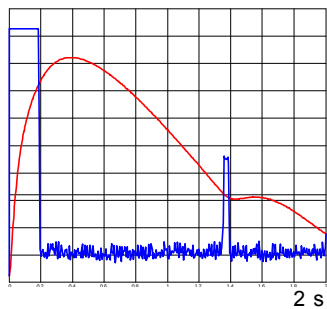
Test No.	Test signal parameters					Evaluation by the analyzer	Graphical presentation of the test signal measured in the IF-output and the associated QP signal relative to the reference indication of the measurement receiver
	1		2		3		
	QP amplitude of impulses adjusted individually relative to QP reference indication of the measurement receiver dB		Duration of impulses ^f adjusted in the intermediate frequency output of the measurement receiver ms		Separation of impulses or periodicity (IF-output) ms		
	Pulse 1	Pulse 2	Pulse 1	Pulse 2			
9	1		0,11		Periodicity 10, min. 21 pulses	Other than click	
10	-2,5	25	30	30	265	1 click	
11	25	-2,5 ^c	190	30	1 034 ^e	2 clicks ^d	
12	25	-2,5 ^c	190	30	1 166 ^e	1 click	

Table 14 (*continued*)

- | | |
|---|---|
| <p>^a</p> <p>^b</p> <p>^c</p> <p>^d</p> <p>^e</p> <p>^f</p> | <p>To be performed with background noise consisting of 200 Hz CISPR pulses at a level 2.5 dB below the quasi-peak threshold level. These pulses should be present commencing at least 1 s before the test pulse and lasting until at least 1 s after the test pulse.</p> <p>Observations:</p> <p>1) The graphical representation is done with peak measurements of a very short hold time (<1 ms) of the test receiver which show the 200-Hz pulse. When the pulse-modulated sine wave arrives, the 200-Hz-pulse is no longer visible (as seen in the graph for test no. 3) but still present during the event of the click disturbance</p> <p>2) The very narrow responses at the origin in the graphs are due to a firmware imperfection.</p> <p>The 1,333 s impulse checks the threshold of the analyzer for impulses, which are only 1 dB above the quasi-peak threshold level.</p> <p>These lower levels shall be set such that the intermediate frequency threshold is exceeded but the quasi-peak threshold is not exceeded</p> <p>If these two pulses were to be measured as separate disturbances, only one click would be registered.</p> <p>The correspondent values for the frequency range above 30 MHz are under consideration and will be revised after further investigations.</p> <p>The rise times of the pulses shall not be longer than 40 µs.</p> |
|---|---|

10.2 Test method for the validation of the performance check for the click analyzer

10.2.1 Basic requirements

The disturbance analyzer is connected to the quasi-peak measuring receiver and tuned to a convenient frequency.

A CW signal and a pulsed CW signal both at the tuned frequency of the receiver are required. A signal generated by CISPR pulse generator, as defined in Annex B, with a 200 Hz PRF covering the receiver bandwidth at the tuned frequency is also required for tests No. 2 and 3.

The pulsed CW signal source shall provide two independently variable pulses. The rise time of the pulses shall be not longer than 40 μ s. The pulse duration shall be variable between 110 μ s and 1,3 s and the amplitudes variable over a 44 dB range. Any background noise of the pulsed CW signal source shall be at least 20 dB below the reference level used in step a) in the test measured on the receiver's quasi-peak meter.

The test procedure is as follows:

- a) The CW signal is connected to the input of the measuring receiver used in conjunction with the disturbance analyzer. The amplitude of the CW signal is adjusted to bring the meter indication to the reference (zero) point on the meter scale of the measuring receiver equal to a value identical to the QP-limit for continuous disturbance. The receiver RF sensitivity (attenuator) control is adjusted to a level above the receiver noise but below the limit for continuous disturbance used as threshold in the IF channel. The corresponding level of the CW signal at the IF output of the receiver constitutes the IF reference level.
- b) The pulsed CW signal is connected to the input of the measuring receiver. For test number 2 and 3 the signal from the CISPR pulse generator is added to the pulsed CW signal. The parameters of the signal are given in Table 14. The amplitudes of the pulses shown in column 1 of Table 14 are adjusted individually relative to the indication of the limit (QP) for continuous disturbance used as threshold in the IF channel. The levels shall be relative to the respective RF and IF reference levels established in the previous paragraph.

10.2.2 Additional requirements

The test method is identical to the one described in 5.4.2.1.

The parameters of the signal are given in Table F.1.

Annex A (normative)

Determination of response to repeated pulses of quasi-peak and r.m.s. measuring receivers (subclauses 3.2, 4.4.2, 7.2.2 and 7.4.1)

A.1 General

This annex sets out the data for the numerical calculation, and the procedure for establishing the curve of response to repeated pulses. The assumptions inherent in the method are also stated. The calculation is divided into three successive stages.

A.2 Response of the pre-detector stages

The pulse response of these stages is, in general, determined solely by the IF stages that define the overall selectivity of the receiver.

It is common practice to consider that this selectivity can be obtained by an assembly of two critically-coupled tuned transformers arranged in cascade so as to produce the desired pass-band at the -6 dB points. Any other equivalent arrangement can be reduced to the above for purposes of calculation. The practical symmetry of this pass-band permits the use of the equivalent low-pass filter for calculating the envelope of the pulse response. The error resulting from this approximation is negligible.

The envelope of the pulse response is written:

$$A(t) = 4 \omega_0 G e^{-\omega_0 t} (\sin \omega_0 t - \omega_0 t \cos \omega_0 t) \quad (\text{A.1a})$$

where

G is the overall gain at tuned frequency;

ω_0 is the angular frequency of value $(\pi/\sqrt{2}) B_6$.

The envelope of the response of two critically-coupled tuned transformers to an impulse area $\omega\tau$ is, from the previous equation:

$$A(t) = (\omega\tau) 4 \omega_0 G e^{-\omega_0 t} (\sin \omega_0 t - \omega_0 t \cos \omega_0 t) \quad (\text{A.1b})$$

The corresponding selectivity curve of the equivalent low-pass filter may be written, for $\tau \ll 1/\omega_0$:

$$F(f) = G \left[\frac{2\omega_0^2}{(\omega_0 + j\omega)^2 + \omega_0^2} \right]^2 \quad (\text{A.2})$$

where

$$\omega = 2\pi f.$$

The bandwidths B_3 and B_6 will be:

$$B_3 = \left[\sqrt{2} \times \sqrt[4]{(\sqrt{2} - 1)} \right] \omega_0 / \pi = 0,361 \omega_0 \quad (\text{A.3a})$$

$$B_6 = \sqrt{2} \times \omega_0 / \pi = 0,450 \omega_0 \quad (\text{A.3b})$$

The effective bandwidth of a receiver, comprising an idealized rectangular filter giving the same r.m.s. value of response as an actual receiver, is equal to the power bandwidth Δf defined as:

$$\Delta f = (1/F_0^2) \int_{-\infty}^{+\infty} F^2(f) df \quad (\text{A.4})$$

where

$F(f)$ is the selectivity curve;

F_0 is the maximum value of $F(f)$ (assuming a single peak selectivity curve).

The power bandwidth is then, for $F_0 = 1$

$$\Delta f = \int_{-\infty}^{+\infty} F^2(f) df \quad (\text{A.5})$$

Taking $F(f)$ from equation (A.2) and putting $G = 1$, we have:

$$\Delta f = \int_0^{\infty} 2 \left[\left(2\omega_0^2 \right) / \left((\omega_0 + j\omega)^2 + \omega_0^2 \right) \right]^4 df \quad (\text{A.6})$$

this leads to:

$$\Delta f = 0,265 \sqrt{2} \times \omega_0 = 0,375 \omega_0 \quad (\text{A.7})$$

thus:

$$B_3 = 0,963 \Delta f \quad (\text{A.8})$$

A.3 Response of the quasi-peak voltmeter detector to output of preceding stages

The calculation is made on the assumption that the connection of the detector circuits to the output of the last IF stages does not affect either the amplitude or the shape of the signal therefrom. In other words, the output impedance of this stage is regarded as negligible compared with the input impedance of the detector.

Any detector may be reduced to the form (actual or equivalent) of a non-linear element (for example a diode) in association with a resistance (total forward resistance S) and followed by a circuit consisting of a capacitance C in shunt with a discharge resistance R .

The electrical charge time constant T_C is related to the product SC , while the electrical discharge time constant T_D is given by the product RC .

The relationship between T_C and the product SC will be established by obtaining, in a time $t = T_C$, an indicated voltage of 0.63 times the final steady value when a constant amplitude RF signal is suddenly applied.

The voltage U across the capacitor is related to the amplitude A of the RF signal applied to the detector by the equation:

$$dU/dt + U/(RC) = A (\sin \theta - \theta \cos \theta)/(\pi \times SC) \quad (A.9)$$

where θ is the conduction angle ($U = A \cos \theta$).

This equation is not directly integrable. A value for the product SC , which, for the time constants chosen satisfies the above conditions, is found by methods of approximation, for example:

in band A:	T_C	=	45 ms
	T_D	=	500 ms
	$2,81SC$	=	1 ms
in band B:	T_C	=	1 ms
	T_D	=	160 ms
	$3,95SC$	=	1 ms
in bands C and D:	T_C	=	1 ms
	T_D	=	550 ms
	$4,07SC$	=	1 ms

By inserting the value thus obtained in equation (A.9), this may be solved for either an isolated pulse or repeated pulses (again by methods of approximation) by introducing, in place of the constant amplitude A , the function $A(t)$ given by equation (A.1) in clause A.2.

This case of repeated pulses can be solved practically only by arbitrarily assuming a level for the output voltage of the detector at the start of each pulse, by determining the increment ΔU of this voltage caused by the pulse, and then finding the spacing which must exist between two successive pulses in order to repeat the assumed initial conditions.

A.3.1 Response of the indicating instrument to the signal from the detector

The only simplifying, but perfectly legitimate, assumption is that the rising portion of the output voltage of the detector is instantaneous.

The following characteristic equation then has to be solved:

$$\frac{d^2\alpha}{dt^2} + \frac{2}{T_M} \frac{d\alpha}{dt} + \frac{1}{T_M^2} \alpha = \frac{1}{T_M^2} \exp\left(\frac{-t}{T_D}\right) \quad (A.10)$$

where

$\alpha(t)$ is the instrument deflection;

T_D is the electrical discharge time constant of the quasi-peak voltmeter;

T_M is the mechanical time constant of the critically damped indicating instrument.

The solution of the problem is relatively simple for the two extremes of the response curve; on the one hand, for pulses sufficiently separated for the starting point to be zero and thus known, and on the other, for pulses having a sufficiently high repetition rate for the inertia of the instrument to prevent it following the fluctuations faithfully. For the intermediate cases, the calculation becomes more complicated. At the start of each pulse, the instrument deflection is varying and it is necessary to find a solution which takes account of the initial position and velocity.

A.4 Response of r.m.s. detector to output voltage of preceding stages

By definition, the output voltage of the r.m.s. detector is given by:

$$U_{\text{rms}} = \left[n \int_0^{+\infty} (A^2(t) / 2) dt \right]^{1/2} \quad (\text{A.11})$$

where

n is the pulse repetition frequency in hertz.

The output may also be deduced from the frequency response curve as:

$$U_{\text{rms}} = \left[n \int_{-\infty}^{+\infty} (2v\tau \times F^2(f) / 2) df \right]^{1/2} \quad (\text{A.12})$$

where

$v\tau$ is the area of pulse having a uniform frequency spectrum.

This gives:

$$U_{\text{rms}} = \sqrt{2} \times v\tau \times \sqrt{n} \left[\int_{-\infty}^{+\infty} F^2(f) df \right]^{1/2} \quad (\text{A.13})$$

Which, from equation (A.5), gives:

$$U_{\text{rms}} = \sqrt{2} \times v\tau \times \sqrt{n} \sqrt{\Delta f} \quad (\text{A.14})$$

From equation (A.14), the amplitude relationship may be deduced by taking:

$$U_{\text{rms}} = 2 \text{ mV, when } n = 100 \text{ Hz}$$

thus:

$$v\tau = (100 \sqrt{2}) / \sqrt{\Delta f} \quad (\mu\text{Vs}) \quad (\text{A.15})$$

or from equation (A.8):

$$v\tau = 139 / \sqrt{B_3} \quad (\mu\text{Vs}) \quad (\text{A.16})$$

A.4.1 Calculation of overload factor

The overload factor corresponding to a pulse repetition frequency of n Hz is calculated as follows:

From equation (A.14):

$$U_{\text{rms}} = (v\tau) \times (2n \Delta f)^{1/2}$$

from equation (A.1), and for $G = 1$:

$$A(t)_{\text{peak}} = 0,944 \times v\tau \times \omega_0$$

thus overload factor:

$$A(t)_{\text{peak}} / \sqrt{2} \times U_{\text{rms}} = 1,28 (B_3/n)^{1/2} \quad (\text{A.17})$$

A.5 Relationship between indication of r.m.s. meter and quasi-peak meter

The amplitude relationship for the r.m.s. meter which states the value of pulse $(v\tau)_{\text{rms}}$ for the case of 100 Hz, which is equivalent to a sine-wave signal of 2 mV is, from equation (A.16):

$$(v\tau)_{\text{rms}} = 139 / \sqrt{B_3} \quad (\mu\text{Vs})$$

For the selectivity characteristic quoted in equation (A.2), this corresponds to:

$$(v\tau)_{\text{rms}} = 155 / \sqrt{B_6} \quad (\mu\text{Vs})$$

when reference is made to the bandwidth at 6 dB.

For the quasi-peak receiver, the value of pulse $(v\tau)_{\text{qp}}$ which is equivalent to a sine-wave signal of 2 mV is as follows:

for the frequency range 0,15 MHz to 30 MHz:

$$(v\tau)_{\text{qp}} = 0,316 \mu\text{Vs}$$

for the frequency range 30 MHz to 1 000 MHz:

$$(v\tau)_{\text{qp}} = 0,044 \mu\text{Vs}$$

Thus for measuring receivers having band-pass characteristics according to equation (A.2) and a bandwidth at 6 dB equal to the nominal bandwidths prescribed in clauses 4, 5, 6 and 7 the following relationships for $(v\tau)_{\text{rms}}/(v\tau)_{\text{qp}}$ exist:

for the frequency range 0,15 MHz to 30 MHz:

$$(v\tau)_{\text{rms}}/(v\tau)_{\text{qp}} = 14,3 \text{ dB}$$

for the frequency range 30 MHz to 1 000 MHz:

$$(v\tau)_{\text{rms}}/(v\tau)_{\text{qp}} = 20,1 \text{ dB}$$

These relationships are valid for a pulse repetition frequency of 100 Hz. At other repetition frequencies, it is necessary to use the corresponding pulse response curves.

Annex B (normative)

Determination of pulse generator spectrum (subclauses 4.4, 5.4, 6.4, 7.4)

B.1 Pulse generator

For checking compliance with the requirements of section 1 of this standard, a pulse generator is needed. Compliance with the requirements of 4.4, 4.6, 5.4, 6.4 and 7.4 may be tested using the pulse generator technique.

For each frequency band of the measuring receiver under test, the generator used shall be capable of producing pulses with the impulse area specified and over the range of repetition frequencies given in table B.1. The impulse area should be known within $\pm 0,5$ dB and the repetition frequency to within about 1 %.

Table B.1 – Pulse generator characteristics

Frequency band of receiver under test	Impulse area μVs	Repetition frequency Hz
0,09 to 0,15 MHz	13,5	1, 2, 5, 10, 25, 60, 100
0,15 to 30 MHz	0,316	1, 2, 10, 20, 100, 1 000
30 to 300 MHz	0,044	1, 2, 10, 20, 100, 1 000
300 to 1 000 MHz	(see note)	1, 2, 10, 20, 100, 1 000
NOTE The generator should be capable of producing pulses of adequate impulse area with as uniform a spectrum up to 1 000 MHz as possible.		

B.1.1 The spectrum of the generated pulses

The spectrum is defined by a curve that represents as a function of the tuned frequency of the receiver under test, the law of variation of the equivalent voltage at the input of a measuring apparatus having a constant bandwidth.

The spectrum should be substantially constant up to the upper limit of the frequency band of the receiver under test. The spectrum may be regarded as satisfactorily uniform if, within this band, the variation of the spectrum amplitude is not greater than 2 dB relative to its value for the lower frequencies within the band. The impulse area at the measurement frequency shall be known to within $\pm 0,5$ dB.

For checking compliance with the requirements of 4.6, the spectrum above the upper limit of the frequency band shall be limited (10 dB down at twice the upper frequency). This is necessary to standardize the severity of the test since the inter-modulation products of all components of the spectrum will contribute to the response.

B.2 General method of measurement

Methods for the accurate determination of the absolute value of the spectrum amplitude of pulses are given in annex C.

For measurement of the variation of the spectrum amplitude with frequency, the following method may be used.

The pulse generator is connected to the input of an RF receiver followed by an oscilloscope connected so as to indicate the RF pulse at the output of the receiver.

At each frequency of tuning of the receiver, the following are measured:

- a) the bandwidth, B_6 Hz, of the receiver at the -6 dB points,
- b) the r.m.s. value, E_0 , of the output from a standard signal generator having the same impedance as the pulse generator and tuned to the mid-band of the receiver and producing on the oscilloscope a deflection equal in amplitude to the peak of the RF pulses.

The relative spectrum amplitude at each frequency is taken to be:

$$S_{\tau}(f) = E_0/B_6$$

The measurement is repeated for various test frequencies in the band under consideration.

The spectrum of the pulse generator is given by the curve relating $S_{\tau}(f)$ to the measurement frequency.

The receiver used should be linear for the peak levels of the signals used.

The suppression of parasitic responses, in particular the image frequency and IF responses, should be at least 40 dB.

The measurements may be made with a receiver conforming to the present specification, using the quasi-peak indicator in place of the oscilloscope, provided that the repetition frequency of the pulses is kept constant throughout the series of measurements.

Annex C (normative)

Accurate measurements of the output of nanosecond pulse generators (subclauses 4.4, 5.4, 6.4, 7.4)

C.1 Measurement of impulse area (IS)

C.1.1 General

Theoretical and practical investigations have shown that, when applied with reasonable care, accurate methods of measurement include those given in C.1.2 to C.1.5.

C.1.2 Area method

The pulses to be measured are fed through a narrow band filter whose passband is centred at frequency f having a symmetrical amplitude characteristic, and an asymmetrical phase characteristic (in conjunction with a filter, an amplifier may be used provided it is operated in its linear range).

The total area under the envelope $A(t, f)$ of the output from the band-pass filter (taking into account the sign of different parts of it) is measured, so as to evaluate the integral in the equation.

$$2(IS) = S(f) = \int_{-\infty}^{+\infty} A(t, f) dt$$

where $S(f)$ is the spectral intensity and $A(t, f)$ is the magnitude of the envelope due to a single isolated pulse (expressed in terms of equivalent input sine-wave voltage).

In applying this equation, the intermediate-frequency amplifier of a low-frequency receiver or a disturbance measuring receiver is used together with a series of frequency converters to tune across the spectrum of the pulse. The output of the final intermediate-frequency amplifier is taken directly to an oscilloscope for the area measurement.

In a variation of this method for pulses of duration much shorter than the period of the frequency (f), the impulse area can be measured directly as an integrated area by means of a suitable oscilloscope (for example, for nanosecond pulses, a sampling oscilloscope is required), the integration taking into account the sign of different parts of the area.

C.1.3 Standard transmission line method

A transmission line of length corresponding to a propagation time τ and charged to a voltage V_0 is discharged into a load resistance equal to the characteristic impedance of the line. The transmission line is considered to consist of the actual line as well as the charged section of the line contained in the switch housing. It has been found that spectral intensity, $S(f)$, has the value $2V_0\tau$ in the low-frequency portion of the spectrum of the resulting pulse in which the amplitude is constant with frequency, this amplitude being independent of the existence of certain stray impedances between the line and the load resistor (e.g. inductance or resistance) or of finite switching time.

C.1.4 Harmonic measurement

This method may be used for pulse generators producing a sequence of pulses with sufficiently high and stable repetition frequency.

When the pulse repetition frequency F exceeds the values of the bandwidth of the measuring receiver, the latter may select one line from the pulse spectrum. In this case, the impulse area may be determined as follows:

$$IS = V_K/2F = V\sqrt{2}/2F$$

where $V_K = V\sqrt{2}$ is the peak value of the k -th harmonic.

The pulse generator may then be used to calibrate the pulse response characteristics of a measuring receiver in which the bandwidth is sufficiently wide to accept many harmonic components (approximately 10 or more within the 6 dB bandwidth).

C.1.5 Energy method

Another method compares the power produced by a thermal source (resistor) with that produced by the pulse generator. However, the accuracy obtained with this method is somewhat less than with the three methods mentioned above. This method may be useful at frequencies of the order of 1 000 MHz.

C.2 Pulse generator spectrum

C.2.1 To determine compliance with 4.4.1, 5.4, 6.4.1 and 7.4.1, the impulse area shall be known with an error not greater than $\pm 0,5$ dB.

C.2.2 The pulse repetition frequency shall be known with an error not greater than 1 %.

C.2.3 For determining compliance with 4.4.2, 5.4, 6.4.2 and 7.4.2 the impulse area shall not depend on their repetition frequency.

C.2.4 For determining compliance with 4.4, 5.4, 6.4 and 7.4 the generator frequency spectrum should be uniform over the pass-band of the measuring receiver. This requirement is considered to be fulfilled in the following cases:

- a) if variation of the frequency spectrum is substantially linear with respect to frequency within the frequency passband of the receiver, and the spectrum irregularity does not exceed 0,5 dB within the receiver passband measured at the -6 dB points;
- b) if the frequency spectrum is smoothly tapered on both sides from the tuning frequency of the receiver, and if the spectrum width at the -6 dB points is at least five times greater than the receiver passband at that level.

In both cases, the impulse area is assumed to be equal to its value at the tuning frequency.

Annex D
(normative)

**Influence of the quasi-peak measuring receiver characteristics
on its pulse response**
(subclause 4.4.2)

The level of the pulse response curve for high repetition frequencies depends essentially on the magnitude of the bandwidth. On the other hand, for low repetition frequencies, the time constants play the more important role. No tolerance has been stated for these time constants, but it is suggested for guidance that a value of 20 % is considered reasonable.

It is also at very low repetition frequencies that the effect of lack of overload factors will be most noticeable. The values required for the overload factors are those necessary for the accurate measurement of an isolated pulse using the bandwidth and the time constants prescribed.

Examination of the pulse response-curve at the two ends of the range of the indicating instrument provides a check on possible non-linear behaviour of the detector. The most critical repetition frequencies in this respect will most probably be in the neighbourhood of 20 Hz to 100 Hz.

Annex E (normative)

Response of average and peak measuring receivers (subclause 6.2.1)

E.1 Response of pre-detector stages

It has been shown* that the area under the envelope of the impulse response curve of a narrowband circuit having a symmetrical frequency characteristic is independent of the bandwidth, and is given by:

$$\int_{-\infty}^{+\infty} A(t) dt = 2 v \tau G_0$$

where v and τ are the amplitude and duration of a rectangular pulse for which $B_{\text{imp}} \tau \ll 1$ and G_0 is the gain of the circuit at the centre frequency.

This theorem is valid only in the case of a non-oscillating envelope. The oscillatory envelope is characteristic of double-tuned circuits, and unless a phase sensitive detector is used, it may be necessary to compensate by calibration the error introduced by the oscillatory response. In the case of critical coupling, the second peak of the envelope is about 8,3 % of the first one.

NOTE The response of the pre-detector stages as defined in clause A.2 is oscillatory. Therefore, the calibration error introduced by the oscillatory response shall be compensated with a biased tolerance of +2,5 dB/−0,5 dB in 6.4.1.

As long as pulses do not overlap in the output of the IF amplifier, the average value is proportional to the pulse repetition rate, n .

Therefore, the average voltage is equal to $2v\tau G_0 n$.

In view of equation (1), it is not considered meaningful to define an effective bandwidth for an average measuring receiver.

E.2 Overload factor

For calculation of overload factor and for use in connection with peak measuring receivers, it is useful to define a quantity known as the effective impulse bandwidth of the pre-detector circuit as follows:

$$B_{\text{imp}} = A(t)_{\text{max}} / 2G_0$$

where

$A(t)_{\text{max}}$ is the peak envelope output of the intermediate-frequency stages with a unit impulse applied.

* "Response of ideal radio noise meter to continuous sine-wave, recurrent impulses, and random noise" by David B. Geselowitz, IRE Transactions, RFI, Vol. RFI-3, no. 1, pp 2-11, May, 1961. See also, "Impulse excitation of a cascade of series tuned circuits" by S. Sabaroff, Proc. IRE, Vol. 32, pp 758-760, December 1944.

From the work leading to equation (A.17) (annex A), we have:

$$B_{\text{imp}} = (0,944/2) \omega_0 = 1,05 B_6 \text{ or } 1,31 B_3$$

where B_6 and B_3 are defined in 3.2.

For other types of tuned circuits, the ratio of B_{imp} to B_6 may be estimated from figure E.1 if the ratio of B_{20} to B_3 is known, where B_{20} is the bandwidth at 20 dB.

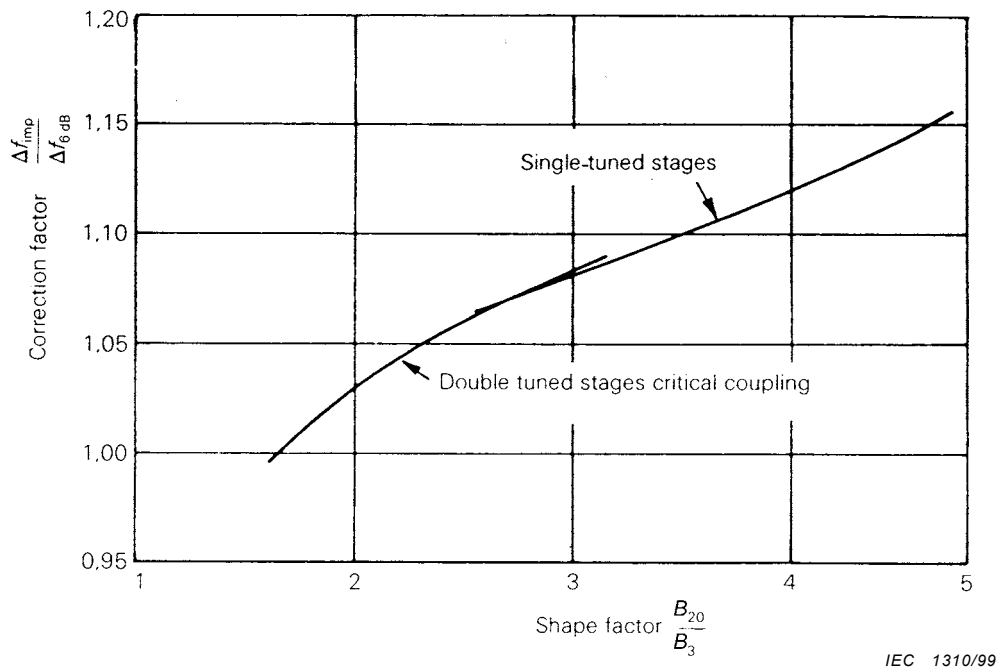


Figure E.1 – Correction factor for estimating the ratio B_{imp}/B_6 for other tuned circuits

E.3 Relationship between indication of an average and a quasi-peak measuring receiver

At a repetition rate of n Hz, the value of impulse area required to produce a response on an average measuring receiver equivalent to the response to an unmodulated sine-wave signal at the tuned frequency of r.m.s. value 2 mV from a signal generator having the same output impedance as the pulse generator is:

$$v\tau = 1,4/n \text{ (mVs)}$$

At a repetition rate of 100 Hz, this is 14 μ Vs.

Therefore, from clause A.5 of annex A, the ratio of $(v\tau)_{\text{ave}}$ to $(v\tau)_{\text{qp}}$ to produce the same indication will be:

for the frequency range 0,15 MHz to 30 MHz:

$$(v\tau)_{\text{ave}}/(v\tau)_{\text{qp}} = 32,9 \text{ dB}$$

for the frequency range 30 MHz to 1 000 MHz:

$$(\nu\tau)_{ave}/(\nu\tau)_{qp} = 50,1 \text{ dB}$$

The above assumes adequate overload factor at the repetition rate in question, and that the bandwidths in use correspond respectively to those in clause 4. At a repetition rate of 1 000 Hz, the corresponding ratios will be 17,4 dB and 38,1 dB.

E.4 Peak measuring receivers

Where a direct-reading meter is used in the receiver, the requirement for time constants can be determined from the curve in figure E.2, which shows the percentage of the reading referred to the true peak in function of a parameter and which includes the time constants ratio, the bandwidth B_6 and the pulse repetition rate. In using this curve, it should be noted that:

$$R_C/R_D = (1/4) (T_C/T_D)$$

where T_C and T_D are respectively the charge and discharge time constants.

For example, if it is desired to have the receiver read at least 90 % of true peak at a repetition rate of 1 Hz, it would be necessary to have a discharge-time constant to charge time constant ratio of:

$1,25 \times 10^6$ in the frequency range 0,15 MHz to 30 MHz;

$1,67 \times 10^7$ in the frequency range 30 MHz to 1 000 MHz.

E.5 Relationship between indication of a peak and a quasi-peak measuring receiver

The value of impulse area, IS , required to produce a response on a peak measuring receiver equivalent to the response to an unmodulated sine-wave signal at the tuned frequency of r.m.s. value 2 mV is:

$$1,4/B_{imp} \text{ (mVs) } (B_{imp} \text{ in Hz})$$

From the 6 dB bandwidths specified in table 1 (4.2), the B_{imp} values are obtained as $1,05B_6$ (clause E.2). These values and the corresponding IS values required for a peak meter will be:

<i>Frequency</i>	<i>IS peak (mVs)</i>	<i>B_{imp} (Hz)</i>
Band A	$6,67 \times 10^{-3}$	$0,21 \times 10^3$
Band B	$0,148 \times 10^{-3}$	$9,45 \times 10^3$
Bands C and D	$0,011 \times 10^{-3}$	126×10^3

Therefore, using the values given as a) in table 2 (in 4.4.1) for IS quasi-peak, the ratio of IS quasi-peak to IS peak to produce the same indication will be:

For Band A 6,1 dB (at 25 Hz pulse repetition frequency)
 For Band B 6,6 dB (at 100 Hz pulse repetition frequency)
 For Bands C and D 12,0 dB (at 1 000 Hz pulse repetition frequency)

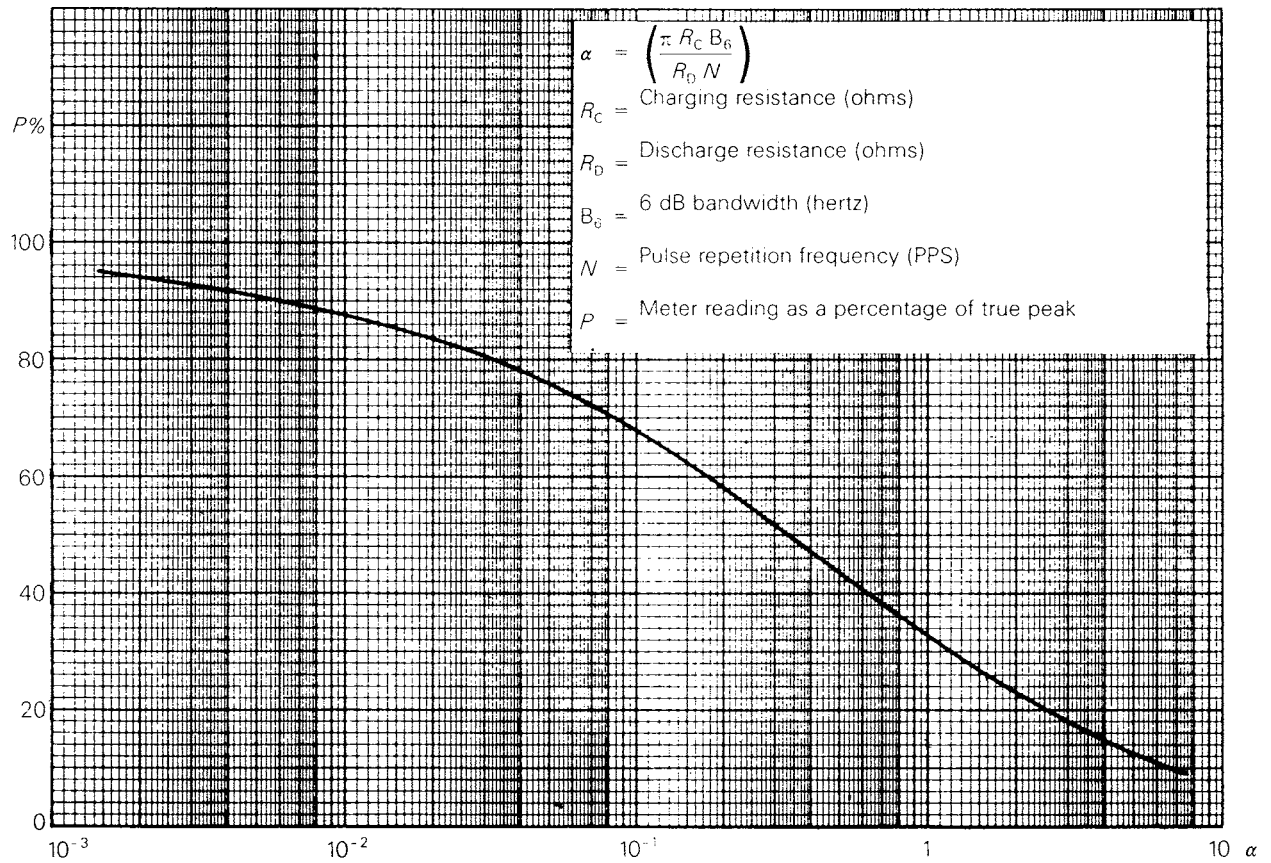


Figure E.2 – Pulse rectification coefficient P

IEC 1311/99

Annex F
(normative)

**Performance check of the exceptions from the definitions of a click
according to 4.2.3 of CISPR 14-1**

For the application of the exceptions given in CISPR 14-1:2000 the disturbance analyzer shall provide the following additional information:

- a) the number of clicks of duration equal to or less than 10 ms;
- b) the number of clicks of duration greater than 10 ms but equal to or less than 20 ms;
- c) the number of clicks of duration greater than 20 ms but equal to or less than 200 ms;
- d) the duration of each registered disturbance the amplitude of which exceeds the QP level limit for cont. disturbance;
- e) an indication that the appliance failed the test, if it is clear that it produces disturbances other than clicks not corresponding to the definition of a click and to which none of the exceptions can be applied;
- f) the time interval from the start of the test to the occurrence of disturbances; mentioned under e);
- g) the total duration of disturbances other than clicks the QP level limit of which exceeds the limit for continuous disturbance;
- h) the click rate.

Table F.1 – Disturbance analyzer test signals^a

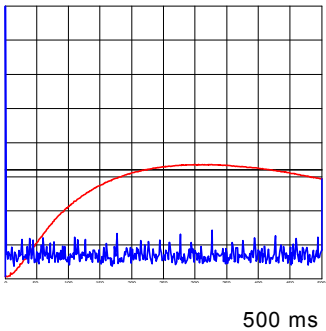
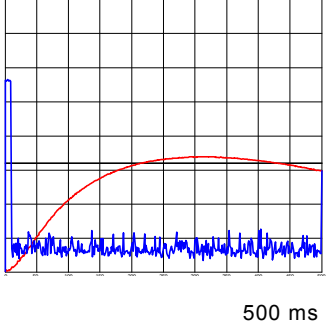
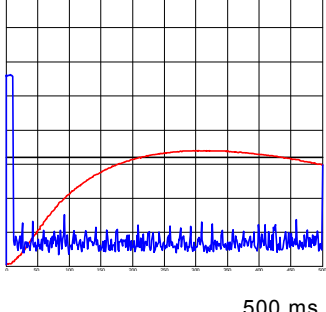
Test No.	Test signal parameters					Evaluation by the analyzer	Graphical presentation of the test signal measured in the IF output and the associated QP signal relative to the reference indication of the measurement receiver
	1		2		3		
	QP Amplitude of impulses adjusted individually relative to QP reference indication of the measurement receiver dB		Duration of impulses ^b adjusted in the intermediate frequency output of the measurement receiver ms		Separation of impulses or periodicity (IF-output) ms		
	Pulse 1	Pulse 2	Pulse 1	Pulse 2			
1	1		0,11			1 click ≤10 ms	
2	1		9,5			1 click ≤10 ms	
3	1		10,5			1 click >10 ms, ≤20 ms	

Table F.1 (continued)

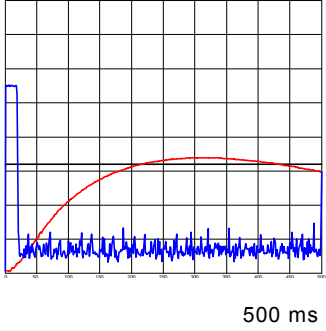
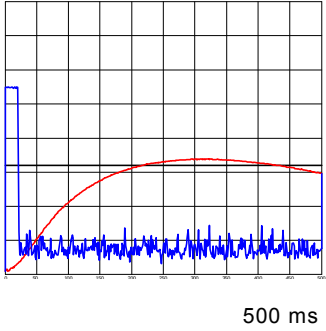
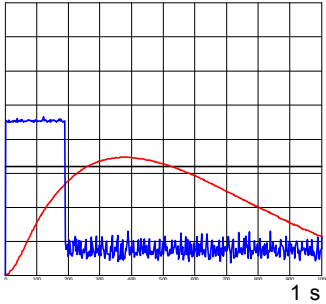
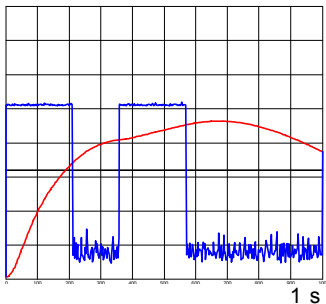
Test No.	Test signal parameters					Evaluation by the analyzer	Graphical presentation of the test signal measured in the IF output and the associated QP signal relative to the reference indication of the measurement receiver
	1		2		3		
	QP Amplitude of impulses adjusted individually relative to QP reference indication of the measurement receiver dB		Duration of impulses ^b adjusted in the intermediate frequency output of the measurement receiver ms		Separation of impulses or periodicity (IF-output) ms		
	Pulse 1	Pulse 2	Pulse 1	Pulse 2			
4	1		19			1 click >10 ms, ≤20 ms	
5	1		21			1 click >20 ms	
6	1		190			1 click >20 ms	
7	5	5	210	210	150	IF only once per program cycle or per minimum observation time: counted as 1 click >20 ms (see NOTE 2, E2, 600 ms rule)	
						OTHERWISE Continuous disturbance (570 ms)	

Table F.1 (continued)

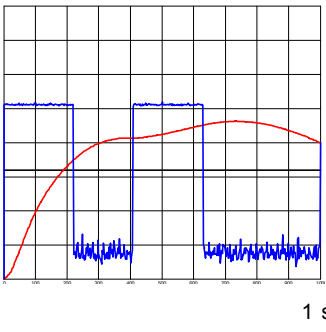
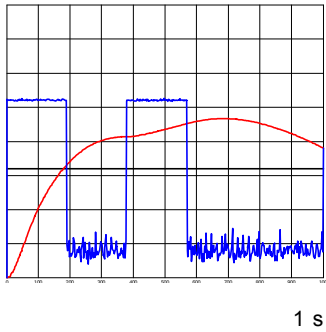
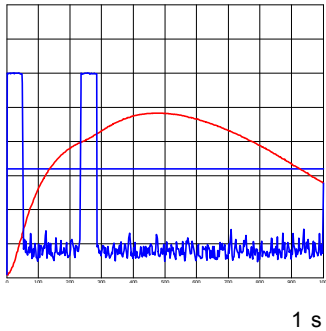
Test No.	Test signal parameters					Evaluation by the analyzer	Graphical presentation of the test signal measured in the IF output and the associated QP signal relative to the reference indication of the measurement receiver
	1		2		3		
	QP Amplitude of impulses adjusted individually relative to QP reference indication of the measurement receiver dB		Duration of impulses ^b adjusted in the intermediate frequency output of the measurement receiver ms		Separation of impulses or periodicity (IF-output) ms		
	Pulse 1	Pulse 2	Pulse 1	Pulse 2			
8	5	5	220	220	190	FAIL Continuous disturbance (See NOTE 2, E2: no exception is applicable because the total duration is 630 ms > 600 ms)	
9	5	5	190	190	190	IF the final click rate is less than 5: 2 clicks >20 ms (see NOTE 2, E4; refrigerator rule; also see NOTE 3)	
						OTHERWISE IF only once per program cycle or once during the minimum observation time: counted as 1 click >20 ms (see NOTE 2, E2) OTHERWISE Fail: continuous disturbance (570 ms)	
10	5	5	50	50	185	IF the final click rate is less than 5: 2 clicks >20 ms (see NOTE 2, E4; also see NOTE 3)	

Table F.1 (continued)

Test No.	Test signal parameters						
	1		2		3	4	5
	QP Amplitude of impulses adjusted individually relative to QP reference indication of the measurement receiver dB		Duration of impulses ^b adjusted in the intermediate frequency output of the measurement receiver ms		Separation of impulses or periodicity (IF-output) ms	Evaluation by the analyzer	Graphical presentation of the test signal measured in the IF output and the associated QP signal relative to the reference indication of the measurement receiver
	Pulse 1	Pulse 2	Pulse 1	Pulse 2			
						OTHERWISE IF not more than once per program cycle or during the minimum observation time: counted as 1 click < 600 ms (see NOTE 2, E2, 2×285 ms >20 ms) OTHERWISE fail: continuous disturbance (285 ms)	
11	20	20	15	5	1 × Pulse 1 + 9 × Pulse 2, repeated until 40 clicks are registered, where the separation between each impulse is 13 s	36 clicks < 10 ms 4 clicks > 10 ms, ≤ 20 ms ≥ 90 % of the clicks < 10 ms PASS (see NOTE 2, E3; also see NOTE 4; a measurement of the click amplitudes is not required.)	
12	20	20	15	5	1 × Pulse 1 + 8 × Pulse 2, repeated until 40 clicks are registered, where the separation between each impulse is 13 s	35 clicks < 10 ms 5 clicks > 10 ms, ≤ 20 ms < 90 % of the clicks < 10 ms (see NOTE 2, E3; also see NOTE 4. No exception is applicable. After application of upper quartile method the final result will be “FAIL” because the click amplitudes are too high.)	

NOTE 1 CISPR 14-1:2000, 4.2.3, contains the following exceptions:

- E1 – “Individual switching operations”
This exception can be evaluated only by the operator, not automatically by the disturbance analyzer. It is mentioned here to avoid confusion with the numbering of the exceptions for users of both CISPR 16-1-1 and CISPR 14-1.
- E2 – “Combination of clicks in a time frame less than 600 ms” (“600 ms rule”)
In program-controlled appliances a combination of clicks in a time frame less than 600 ms is allowed once per selected program cycle. For other appliances such a combination of clicks is allowed once during the minimum observation time. This is also valid for thermostatically controlled three-phase switches, causing three disturbances sequentially in each of the three phases and the neutral. The combination of clicks is considered as one click.

- E3 – “Instantaneous switching”
Appliances which fulfil the following conditions:
 - the click rate is not more than 5,
 - none of the caused clicks has a duration longer than 20 ms, and
 - 90% of the caused clicks have a duration less than 10 ms,
 shall be deemed to comply with the limits, independent of the amplitude of the clicks. If one of these conditions is not satisfied then the limits for discontinuous disturbance apply.
- E4 – “Separation of clicks less than 200 ms” (refrigerator rule)
For appliances which have a click rate less than 5, any two disturbances each having a maximum duration of 200 ms, shall be evaluated as two clicks even when the separation between the disturbances is less than 200 ms. In this case, for instance observed with refrigerators, such a configuration has to be evaluated as two clicks and not as a continuous disturbance.

NOTE 2 The analyzer has to apply exception E2 only if E4 is not applicable.






NOTE 3 The check wave forms 11 and 12 can pass the test only in case exception E3 can be applied, as the following calculation shows:

- Including the click at “0” seconds for the check wave forms 11 and 12, the required 40 clicks will be counted after $13 \text{ s} \times 39 = 507 \text{ s}$, i.e. 8,45 min. The click rate is $40 / 8,45 = 4,734$ (less than 5 as required – here all depends on whether 90 % are <10 ms or not).

NOTE 4 The relaxation of the limit for the clicks according to CISPR 14-1 is: $20 \times \log (30 / 4,734) = 16,04 \text{ [dB]}$. Therefore the check waveforms 11 and 12 (amplitude 20 dB over the limit) never can pass the upper quartile check according to CISPR 14-1:2000, which means that no more than 25 % of the clicks are allowed to exceed the click limit.

^a Test signals used for the performance check with the evaluation of the exceptions from the definition of a click according to CISPR 14-1:2000, 4.2.3.

^b The rise times of the pulses shall not be longer than 40 μs .

Test No	Test signal	Evaluation by the analyzer
1	 0,11 m/1 dB	1 click ≤10 ms
2	 9,5 ms/1 dB	1 click ≤10 ms
3	 10,5 ms/1 dB	1 click >10 ms, ≤20 ms
4	 19 ms/1 dB	1 click > 10 ms, ≤20 ms
5	 21 ms/1 dB	1 click >20 ms
6	 190 ms/1 dB	1 click >20 ms
7	 210 ms/5 dB 150 ms 210 ms/5 dB	1 click ≤600 ms (DUT programme-controlled)
8	 220 ms/5 dB 190 ms 220 ms/5 dB	Continuous ≥600 ms
9	 190 ms/5 dB 190 ms 190 ms/5 dB	1 click ≤600 ms (counted as 2 clicks refrigerator rule)
10	 50 ms/5 dB 185 ms 50 ms/5 dB	for N <5 - 2 clicks for N ≥5 - continuous, or 1 click ≤600 ms for programme controlled DUT
11	 15 ms/20 dB 13 s 13 s 13 s 13 s 13 s 13 s 13 s 13 s 13 s 9 pulses/5 ms/20 dB repeated up to 40 counted clicks	36 clicks ≤10 ms 4 clicks >10 ms, ≤20 ms
12	 15 ms/20 dB 13 s 13 s 13 s 13 s 13 s 13 s 13 s 13 s 8 pulses/5 ms/20 dB repeated up to 40 counted clicks	35 clicks <10 ms 5 clicks >10 ms, ≤20 ms

IEC 1124/03

Figure F.1 – A graphical presentation of the test signals used for the performance check of the analyzer with the additional requirements according to Table F.1

FOREWORD

This amendment has been prepared by CISPR subcommittee A: Radio interference measurements and statistical methods.

The text of this amendment is based on the following documents:

FDIS	Report on voting
CISPR/A/579/FDIS	CISPR/A/593/RVD

Full information on the voting for the approval of this amendment can be found in the report on voting indicated in the above table.

The committee has decided that the contents of this amendment and the base publication will remain unchanged until the maintenance result date indicated on the IEC web site under "<http://webstore.iec.ch>" in the data related to the specific publication. At this date, the publication will be

- reconfirmed,
- withdrawn,
- replaced by a revised edition, or
- amended.

Page 59

8.2 Spectrum analysers and scanning receivers for the frequency range 1 GHz to 18 GHz

Add, after item g) on page 61, the following new item:

h) Amplitude probability distribution (APD) measuring function

APD of disturbance is defined as the cumulative distribution of the "probability of time that the amplitude of disturbance exceeds a specified level".

APD can be measured at the output of the envelope detector or the succeeding circuits of an RF measuring receiver or a spectrum analyzer. The amplitude of disturbance should be expressed in terms of the corresponding field strength or voltage at the receiver input. Usually, an APD measurement is carried out at a fixed frequency.

The APD measuring function will be an additional function of the measuring apparatus and may be attached to, or incorporated in the measuring instrument.

The APD measuring function can be implemented using the following methods. One approach uses comparators and counters (Figure G.1). The equipment determines the probabilities of exceeding a set of pre-assigned amplitude (i.e. voltage) levels. The number of levels equals the number of comparators. Another possible method involves the use of an analog-to-digital converter, a logic circuit, and memory (Figure G.2). The equipment can also provide the APD figure for a set of pre-assigned amplitude levels. The number of levels depends on the resolution of the analog-to-digital converter (e.g. 256 levels for an 8-bit converter).

APD measurements using the aforementioned function are applicable to products or product families if their potential to cause interference to digital communication systems is to be determined (see CISPR 16-3, Amendment 1¹⁾, subclause 4.7, for background material to amplitude probability distribution (APD) specifications).

The following specifications apply to the APD measuring function. A rationale for these specifications is provided in Annex G.

- **Specifications**

- a) The dynamic range of the amplitude shall be greater than 60 dB.
- b) The amplitude accuracy, including threshold level setting error, shall be better than $\pm 2,7$ dB.
- c) The maximum measurable time of a disturbance shall be longer than or equal to 2 min. The intermittent measurement can be used if the dead time is less than 1 % of the total measurement time.
- d) The minimum measurable probability shall be 10^{-7} .
- e) The APD measuring function shall be capable of assigning at least two amplitude levels. The probabilities corresponding to all pre-assigned levels shall be measured simultaneously. The resolution of the pre-assigned amplitude levels shall be 0,25 dB at a minimum or better
- f) The sampling rate shall be greater than or equal to 10 million samples per second when using a resolution bandwidth of 1 MHz.

- **Recommended specification**

- g) The amplitude resolution of the APD display should be less than 0,25 dB for APD measuring equipment with an A/D converter.

NOTE APD measurements may also be applicable in the frequency range below 1 GHz.

Annex G (informative)

Rationale for the specifications of the APD measuring function

The specifications are based on the following definitions and considerations:

a) Dynamic range of the amplitude

The dynamic range of the amplitude is defined as the range necessary to obtain the APD. The upper limit of the dynamic range shall be greater than the peak level of disturbance to be measured and the lower limit shall be lower than the level of disturbance limit specified by the product committees.

According to CISPR 11, the peak limit for group 2, class B, for ISM equipment is set at 110 dB μ V/m, and the weighted limit is specified as 60 dB μ V/m. Therefore, a dynamic range of greater than 60 dB is proposed, with a 10 dB margin.

b) Sampling rate

Ideally, the APD of disturbances is measured using the equivalent bandwidth of the radio service to be protected. However, the spectrum analyzer's resolution bandwidth is specified as 1 MHz for the frequency range above 1 GHz. The sampling rate shall therefore be greater than 10 million samples per second.

c) Maximum measurable time

CISPR 11 specifies the maximum hold time as a 2 min period for peak measurements of microwave cooking appliances above 1 GHz. Therefore, the measurable time for an APD measurement shall be 2 min minimum. Because the size of the counter or memory is limited, continuous measurements may be difficult for long measurement periods. Therefore, intermittent measurements are allowed under the condition that the dead time is less than 1 % of the total measurement time.

d) Minimum measurable probability

About 100 occurrences may be necessary to obtain a meaningful result. Therefore, the minimum measurable probability is calculated as follows:

assuming 2 min for the measuring time and a 10 million samples per second sampling rate, the probability is determined as:

$$100/(120 \times 10 \times 10^6) \sim 10^{-7}$$

e) Display of APD measurement data

The amplitude resolution for the display of APD results depends on the dynamic range and the resolution of the A/D converter. For example, the resolution of the display comes to less than 0,25 dB ($\sim 60 \text{ dB}/256$) when an 8-bit A/D converter is applied to a dynamic range of 60 dB.

Figures G.1 and G.2 show block diagrams of implementations of the APD measurement function.

An example of an APD measurement result is depicted in Figure G.3.

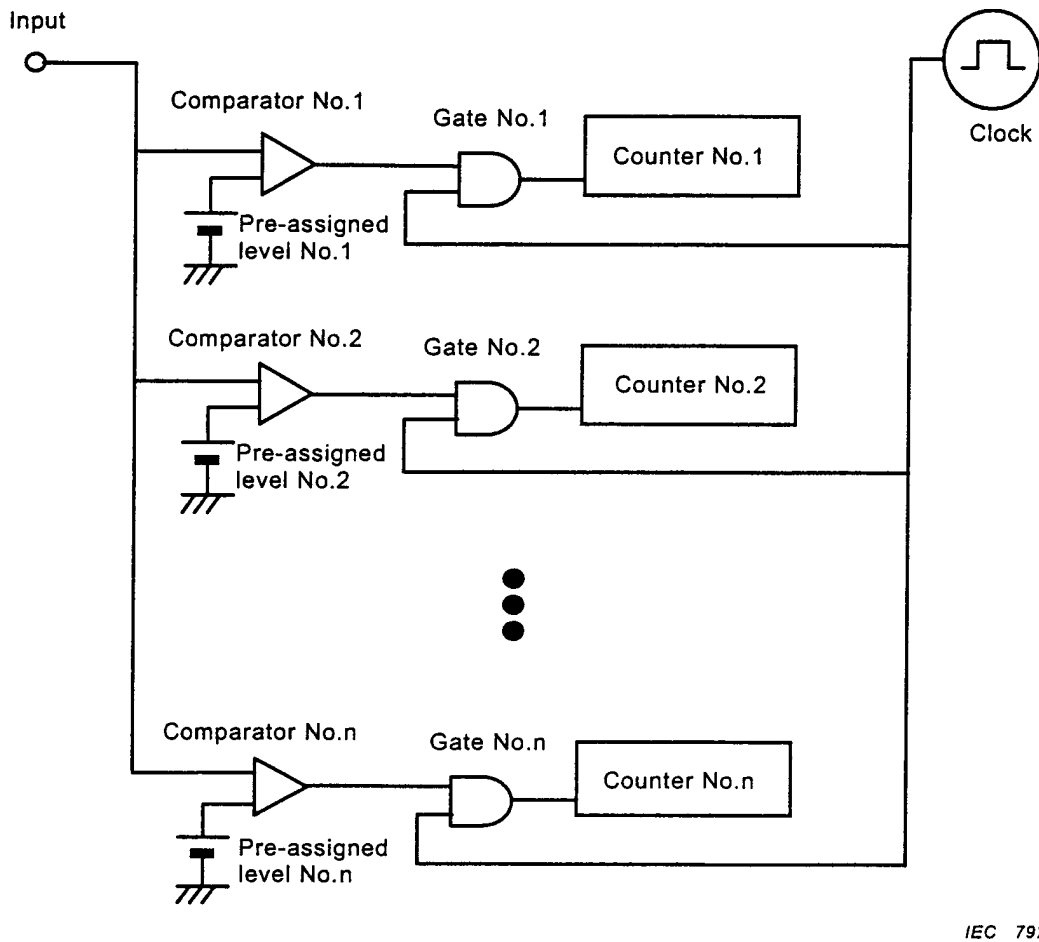


Figure G.1 – Block diagram of APD measurement circuit without A/D converter

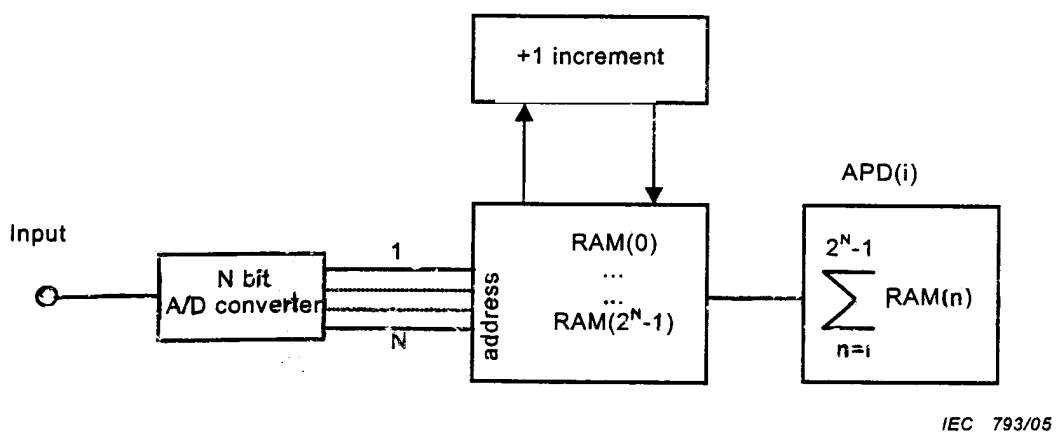


Figure G.2 – Block diagram of APD measurement circuit with A/D converter

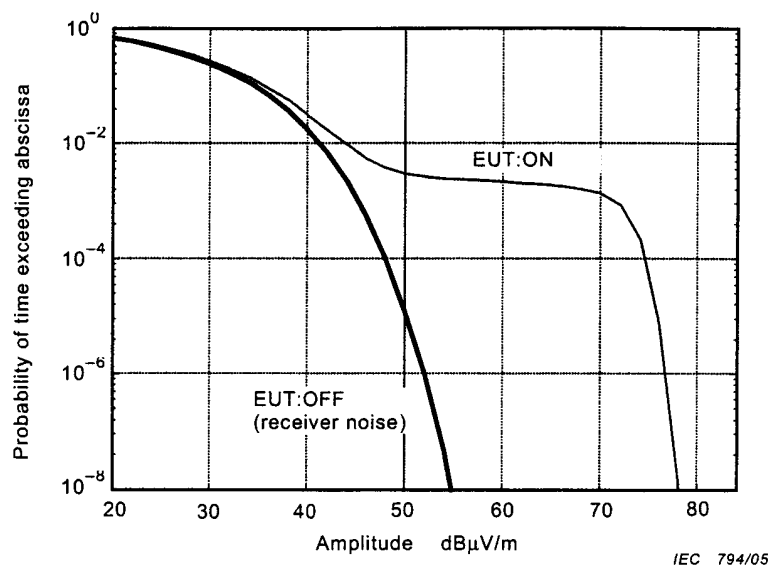


Figure G.3 – Example of display of APD measurement